

# Technical Information

## Proline Promag H 300

Electromagnetic flowmeter



The specialist for hygienic applications with a compact, easily accessible transmitter

### Application

- The bidirectional measuring principle is virtually independent of pressure, density, temperature and viscosity
- Dedicated to demanding applications in the food and beverage as well as in life sciences industries

### Device properties

- Liner made of PFA
- Sensor housing made of stainless steel (3-A, EHEDG)
- Wetted materials CIP/SIP cleanable
- Compact hygienic dual-compartment housing with IP69 and up to 3 I/Os
- Backlit display with touch control and WLAN access
- Remote display available

### Your benefits

- Flexible installation concept – numerous hygienic process connections
- Energy-saving flow measurement – no pressure loss due to cross-section constriction
- Maintenance-free – no moving parts
- Full access to process and diagnostic information – numerous, freely combinable I/Os and fieldbuses
- Reduced complexity and variety – freely configurable I/O functionality
- Integrated verification – Heartbeat Technology

## Table of contents






<b>About this document</b> . . . . .	<b>4</b>	Impact resistance . . . . .	46
Symbols used . . . . .	4	Mechanical load . . . . .	46
<b>Function and system design</b> . . . . .	<b>5</b>	Interior cleaning . . . . .	46
Measuring principle . . . . .	5	Electromagnetic compatibility (EMC) . . . . .	46
Measuring system . . . . .	6	<b>Process</b> . . . . .	<b>47</b>
Equipment architecture . . . . .	7	Medium temperature range . . . . .	47
Safety . . . . .	7	Conductivity . . . . .	47
<b>Input</b> . . . . .	<b>9</b>	Pressure-temperature ratings . . . . .	47
Measured variable . . . . .	9	Pressure tightness . . . . .	53
Measuring range . . . . .	9	Flow limit . . . . .	53
Operable flow range . . . . .	10	Pressure loss . . . . .	53
Input signal . . . . .	10	System pressure . . . . .	54
<b>Output</b> . . . . .	<b>12</b>	Vibrations . . . . .	55
Output and input variants . . . . .	12	<b>Mechanical construction</b> . . . . .	<b>55</b>
Output signal . . . . .	13	Dimensions in SI units . . . . .	55
Signal on alarm . . . . .	16	Dimensions in US units . . . . .	74
Ex connection data . . . . .	19	Weight . . . . .	87
Low flow cut off . . . . .	20	Measuring tube specification . . . . .	88
Galvanic isolation . . . . .	20	Materials . . . . .	88
Protocol-specific data . . . . .	20	Fitted electrodes . . . . .	90
<b>Power supply</b> . . . . .	<b>25</b>	Process connections . . . . .	90
Terminal assignment . . . . .	25	Surface roughness . . . . .	90
Device plugs available . . . . .	25	<b>Operability</b> . . . . .	<b>90</b>
Pin assignment, device plug . . . . .	26	Operating concept . . . . .	90
Supply voltage . . . . .	28	Languages . . . . .	91
Power consumption . . . . .	28	Local operation . . . . .	91
Current consumption . . . . .	28	Remote operation . . . . .	92
Power supply failure . . . . .	28	Service interface . . . . .	97
Electrical connection . . . . .	29	Network integration . . . . .	98
Potential equalization . . . . .	37	Supported operating tools . . . . .	99
terminals . . . . .	39	HistoROM data management . . . . .	100
Cable entries . . . . .	39	<b>Certificates and approvals</b> . . . . .	<b>102</b>
Cable specification . . . . .	39	CE mark . . . . .	102
<b>Performance characteristics</b> . . . . .	<b>41</b>	C-Tick symbol . . . . .	102
Reference operating conditions . . . . .	41	Ex approval . . . . .	102
Maximum measured error . . . . .	41	Sanitary compatibility . . . . .	103
Repeatability . . . . .	42	Pharmaceutical compatibility . . . . .	103
Temperature measurement response time . . . . .	42	Functional safety . . . . .	103
Influence of ambient temperature . . . . .	42	HART certification . . . . .	103
<b>Installation</b> . . . . .	<b>43</b>	FOUNDATION Fieldbus certification . . . . .	103
Mounting location . . . . .	43	Certification PROFIBUS . . . . .	103
Orientation . . . . .	43	EtherNet/IP certification . . . . .	103
Inlet and outlet runs . . . . .	44	Certification PROFINET . . . . .	104
Adapters . . . . .	45	Radio approval . . . . .	104
<b>Environment</b> . . . . .	<b>46</b>	Pressure Equipment Directive . . . . .	104
Ambient temperature range . . . . .	46	Measuring instrument approval . . . . .	104
Storage temperature . . . . .	46	Additional certification . . . . .	104
Degree of protection . . . . .	46	Other standards and guidelines . . . . .	104
Vibration resistance . . . . .	46	<b>Ordering information</b> . . . . .	<b>105</b>
Shock resistance . . . . .	46	<b>Application packages</b> . . . . .	<b>105</b>
		Diagnostics functions . . . . .	105

Heartbeat Technology . . . . .	106
Cleaning . . . . .	106
OPC-UA server . . . . .	106
<b>Accessories . . . . .</b>	<b>106</b>
Device-specific accessories . . . . .	106
Communication-specific accessories . . . . .	107
Service-specific accessories . . . . .	108
System components . . . . .	109
<b>Supplementary documentation . . . . .</b>	<b>109</b>
Standard documentation . . . . .	109
Device-dependent additional documentation . . . . .	109
<b>Registered trademarks . . . . .</b>	<b>110</b>





## About this document

### Symbols used









#### Electrical symbols

Symbol	Meaning
	Direct current
	Alternating current
	Direct current and alternating current
	<b>Ground connection</b> A grounded terminal which, as far as the operator is concerned, is grounded via a grounding system.
	<b>Protective Earth (PE)</b> A terminal which must be connected to ground prior to establishing any other connections.  The ground terminals are situated inside and outside the device: <ul style="list-style-type: none"> <li>■ Inner ground terminal: Connects the protective earth to the mains supply.</li> <li>■ Outer ground terminal: Connects the device to the plant grounding system.</li> </ul>

#### Communication symbols




Symbol	Meaning
	<b>Wireless Local Area Network (WLAN)</b> Communication via a wireless, local network.
	<b>LED</b> Light emitting diode is off.
	<b>LED</b> Light emitting diode is on.
	<b>LED</b> Light emitting diode is flashing.

#### Symbols for certain types of information

Symbol	Meaning
	<b>Permitted</b> Procedures, processes or actions that are permitted.
	<b>Preferred</b> Procedures, processes or actions that are preferred.
	<b>Forbidden</b> Procedures, processes or actions that are forbidden.
	<b>Tip</b> Indicates additional information.
	Reference to documentation.
	Reference to page.
	Reference to graphic.
	Visual inspection.




Symbols in graphics

Symbol	Meaning
1, 2, 3, ...	Item numbers
1, 2, 3, ...	Series of steps
A, B, C, ...	Views
A-A, B-B, C-C, ...	Sections
	Hazardous area
	Safe area (non-hazardous area)
	Flow direction

Function and system design

Measuring principle

Following *Faraday's law of magnetic induction*, a voltage is induced in a conductor moving through a magnetic field.

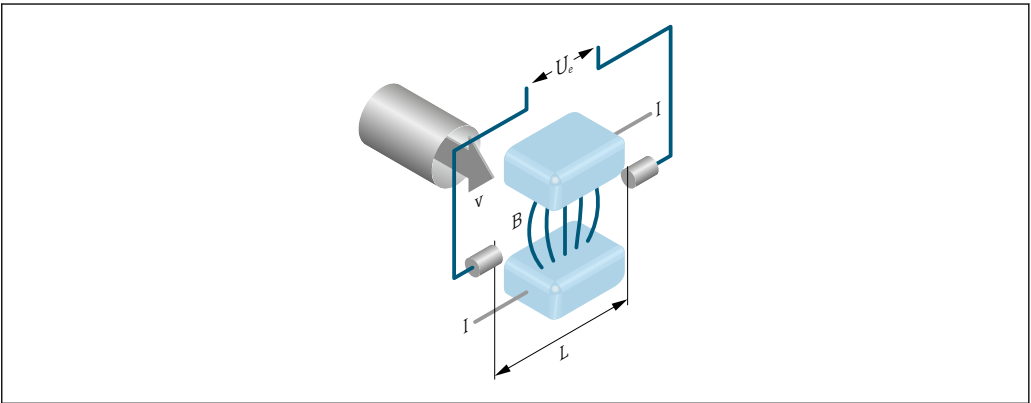

- U<sub>e</sub>* Induced voltage
- B* Magnetic induction (magnetic field)
- L* Electrode spacing
- I* Current
- v* Flow velocity

In the electromagnetic measuring principle, the flowing medium is the moving conductor. The voltage induced (*U<sub>e</sub>*) is proportional to the flow velocity (*v*) and is supplied to the amplifier by means of two measuring electrodes. The flow volume (*Q*) is calculated via the pipe cross-section (*A*). The DC magnetic field is created through a switched direct current of alternating polarity.

Formulae for calculation

- Induced voltage  $U_e = B \cdot L \cdot v$
- Volume flow  $Q = A \cdot v$


**Measuring system**

The device consists of a transmitter and a sensor.



The device is available as a compact version:

The transmitter and sensor form a mechanical unit.


**Transmitter**

<p><b>Promag 300</b></p>  <p>A0026708</p>	<p>Device versions and materials:</p> <ul style="list-style-type: none"> <li>■ Transmitter housing           <ul style="list-style-type: none"> <li>– Aluminum, coated: aluminum, AlSi10Mg, coated</li> <li>– Stainless, hygienic: stainless steel, 1.4404</li> </ul> </li> <li>■ Material of window in transmitter housing:           <ul style="list-style-type: none"> <li>– Aluminum, coated: glass</li> <li>– Stainless, hygienic: polycarbonate</li> </ul> </li> </ul> <p>With order code for "Approval", option <b>BS, CZ, GS, MS</b> and <b>NS</b>: glass</p> <p>Configuration:</p> <ul style="list-style-type: none"> <li>■ External operation via 4-line, backlit, graphic local display with touch control and guided menus ("Make-it-run" wizards) for application-specific commissioning.</li> <li>■ Via service interface or WLAN interface:           <ul style="list-style-type: none"> <li>– Operating tools (e.g. FieldCare, DeviceCare, SmartBlue app)</li> <li>– Web server (access via Web browser, e.g. Microsoft Internet Explorer, Microsoft Edge)</li> </ul> </li> </ul>
--	---

**Sensor**

<p><b>Promag H</b></p>  <p>A0028964</p>  <p>A0028965</p>	<p>Nominal diameter range: DN 2 to 150 (1/12 to 6")</p> <p>Materials:</p> <ul style="list-style-type: none"> <li>■ Sensor housing: stainless steel, 1.4301 (304)</li> <li>■ Measuring tubes: stainless steel, 1.4301 (304)</li> <li>■ Liner: PFA</li> <li>■ Electrodes: stainless steel, 1.4435 (316L); Alloy C22, 2.4602 (UNS N06022); tantalum; platinum (only up to DN 25 (1"))</li> <li>■ Process connections: stainless steel, 1.4404 (F316L); PVDF; PVC adhesive sleeve</li> <li>■ Seals:           <ul style="list-style-type: none"> <li>– DN 2 to 25 (1/12 to 1"): O-ring seal (EPDM, FKM, Kalrez), aseptic gasket seal (EPDM, FKM, silicone)</li> <li>– DN 40 to 150 (1 1/2 to 6"): aseptic gasket seal (EPDM, FKM, silicone)</li> </ul> </li> <li>■ Grounding rings: stainless steel, 1.4435 (316L); Alloy C22, 2.4602 (UNS N06022); tantalum</li> </ul>
--	---

Equipment architecture

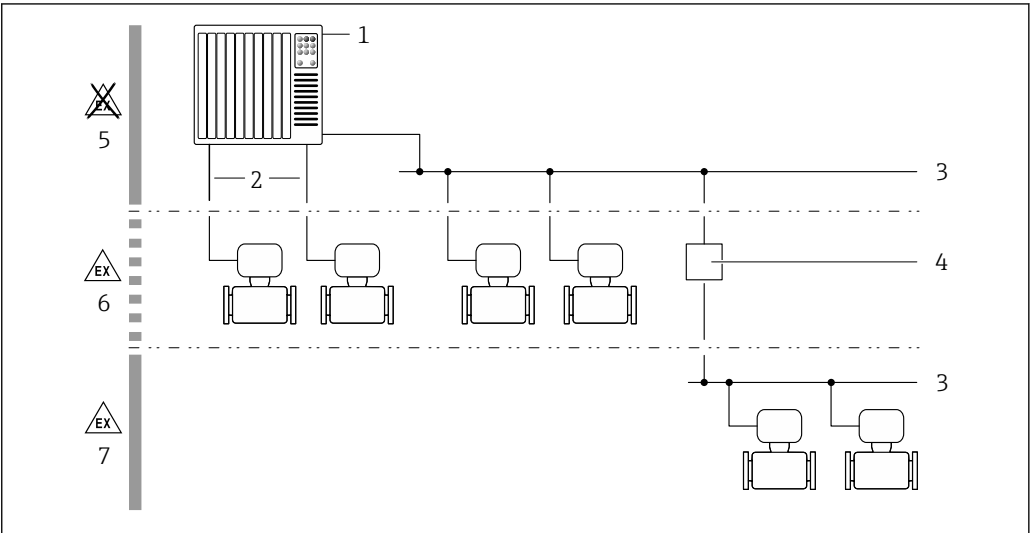

A0027512

1 Possibilities for integrating measuring devices into a system

- 1 Control system (e.g. PLC)
- 2 Connecting cable (0/4 to 20 mA HART etc.)
- 3 Fieldbus
- 4 Segment coupler
- 5 Non-hazardous area
- 6 Hazardous area: Zone 2; Class I, Division 2
- 7 Hazardous area: Zone 1; Class I, Division 1

Safety

IT security

We only provide a warranty if the device is installed and used as described in the Operating Instructions. The device is equipped with security mechanisms to protect it against any inadvertent changes to the device settings.



IT security measures in line with operators' security standards and designed to provide additional protection for the device and device data transfer must be implemented by the operators themselves.

Device-specific IT security

The device offers a range of specific functions to support protective measures on the operator's side. These functions can be configured by the user and guarantee greater in-operation safety if used correctly. An overview of the most important functions is provided in the following section.

For detailed information on device-specific IT security, see the Operating Instructions for the device

Function/interface	Factory setting	Recommendation
Write protection via hardware write protection switch → 8	Not enabled.	On an individual basis following risk assessment.
Access code (also applies for Web server login or FieldCare connection) → 8	Not enabled (0000).	Assign a customized access code during commissioning.
WLAN (order option in display module)	Enabled.	On an individual basis following risk assessment.
WLAN security mode	Enabled (WPA2-PSK)	Do not change.
WLAN passphrase (password) → 8	Serial number	Assign a customized access code during commissioning.
WLAN mode	Access Point	On an individual basis following risk assessment.

Function/interface	Factory setting	Recommendation
Web server →  8	Enabled.	On an individual basis following risk assessment.
CDI-RJ45 service interface →  9	–	On an individual basis following risk assessment.

#### *Protecting access via hardware write protection*

Write access to the device parameters via the local display, Web browser or operating tool (e.g. FieldCare, DeviceCare) can be disabled via a write protection switch (DIP switch on the motherboard). When hardware write protection is enabled, only read access to the parameters is possible.

Hardware write protection is disabled when the device is delivered.

#### *Protecting access via a password*

Different passwords are available to protect write access to the device parameters or access to the device via the WLAN interface.

- **User-specific access code**  
Protect write access to the device parameters via the local display, Web browser or operating tool (e.g. FieldCare, DeviceCare). Access authorization is clearly regulated through the use of a user-specific access code.
- **WLAN passphrase**  
The network key protects a connection between an operating unit (e.g. notebook or tablet) and the device via the WLAN interface which can be ordered as an option.

#### *User-specific access code*

Write access to the device parameters via the local display, Web browser or operating tool (e.g. FieldCare, DeviceCare) can be protected by the modifiable, user-specific access code.

#### *WLAN passphrase*

A connection between an operating unit (e.g. notebook or tablet) and the device via the WLAN interface which can be ordered as an option is protected by the network key. The WLAN authentication of the network key complies with the IEEE 802.11 standard.

When the device is delivered, the network key is pre-defined depending on the device. It can be changed via the **WLAN settings** submenu in the **WLAN passphrase** parameter.

#### *General notes on the use of passwords*


- The access code and network key supplied with the device should be changed during commissioning.
- Follow the general rules for generating a secure password when defining and managing the access code or network key.
- The user is responsible for the management and careful handling of the access code and network key.

#### *Access via fieldbus*

When communicating via fieldbus, access to the device parameters can be restricted to "Read only" access. The option can be changed in the **Fieldbus writing access** parameter.

This does not affect cyclic measured value transmission to the higher-order system, which is always guaranteed.



For detailed information, see the "Description of Device Parameters" document pertaining to the device →  109

#### *Access via Web server*

The device can be operated and configured via a Web browser with the integrated Web server. The connection is via the service interface (CDI-RJ45) or the WLAN interface. For device versions with the EtherNet/IP and PROFINET communication protocols, the connection can also be established via the terminal connection for signal transmission with EtherNet/IP or PROFINET (RJ45 connector).

The Web server is enabled when the device is delivered. The Web server can be disabled if necessary (e.g. after commissioning) via the **Web server functionality** parameter.

The device and status information can be hidden on the login page. This prevents unauthorized access to the information.



For detailed information, see the "Description of Device Parameters" document pertaining to the device → 109

#### Access via CDI-RJ45 service interface

The device can be connected to a network via the CDI-RJ45 service interface. Device-specific functions guarantee the secure operation of the device in a network.

It is advisable to take relevant security concepts into consideration, such as those issued by the Federal Office for Information Security. This includes organizational security measures such as the assignment of access authorization as well as technical measures such as network segmentation.



The device can be integrated in a ring topology. The device is integrated via the terminal connection for signal transmission (output 1) and the connection to the service interface (CDI-RJ45) → 95.

## Input

### Measured variable

#### Direct measured variables

- Volume flow (proportional to induced voltage)
- Temperature (DN 15 to 150 (½ to 6"))
- Electrical conductivity

#### Calculated measured variables

- Mass flow
- Corrected volume flow
- Corrected electrical conductivity

### Measuring range

Typically  $v = 0.01$  to  $10$  m/s ( $0.03$  to  $33$  ft/s) with the specified accuracy

#### Flow characteristic values in SI units

Nominal diameter		Recommended flow min./max. full scale value ( $v \sim 0.3/10$ m/s)	Factory settings		
[mm]	[in]		Full scale value current output ( $v \sim 2.5$ m/s)	Pulse value ( $\sim 2$ pulse/s)	Low flow cut off ( $v \sim 0.04$ m/s)
		[dm <sup>3</sup> /min]	[dm <sup>3</sup> /min]	[dm <sup>3</sup> ]	[dm <sup>3</sup> /min]
2	1/12	0.06 to 1.8	0.5	0.005	0.01
4	5/32	0.25 to 7	2	0.025	0.05
8	5/16	1 to 30	8	0.1	0.1
15	½	4 to 100	25	0.2	0.5
25	1	9 to 300	75	0.5	1
40	1 ½	25 to 700	200	1.5	3
50	2	35 to 1 100	300	2.5	5
65	–	60 to 2 000	500	5	8
80	3	90 to 3 000	750	5	12
100	4	145 to 4 700	1200	10	20
125	5	220 to 7 500	1850	15	30
150	6	20 to 600 m <sup>3</sup> /h	150 m <sup>3</sup> /h	0.03 m <sup>3</sup>	2.5 m <sup>3</sup> /h

*Flow characteristic values in US units*

Nominal diameter		Recommended flow  min./max. full scale value (v ~ 0.3/10 m/s)	Factory settings		
			Full scale value current output (v ~ 2.5 m/s)	Pulse value (~ 2 pulse/s)	Low flow cut off (v ~ 0.04 m/s)
[in]	[mm]	[gal/min]	[gal/min]	[gal]	[gal/min]
1/12	2	0.015 to 0.5	0.1	0.001	0.002
5/32	4	0.07 to 2	0.5	0.005	0.008
5/16	8	0.25 to 8	2	0.02	0.025
½	15	1 to 27	6	0.05	0.1
1	25	2.5 to 80	18	0.2	0.25
1 ½	40	7 to 190	50	0.5	0.75
2	50	10 to 300	75	0.5	1.25
3	80	24 to 800	200	2	2.5
4	100	40 to 1250	300	2	4
5	125	60 to 1950	450	5	7
6	150	90 to 2 650	600	5	12



To calculate the measuring range, use the *Applicator* sizing tool → 108

**Recommended measuring range**

"Flow limit" section → 53



For custody transfer, the applicable approval determines the permitted measuring range, the pulse value and the low flow cut off.

**Operable flow range**

Over 1000 : 1



For custody transfer, the operable flow range is 100 : 1 to 250 : 1, depending on the nominal diameter. Further details are specified by the applicable approval.

**Input signal****Input and output versions**

→ 12

**External measured values**

To increase the accuracy of certain measured variables or to calculate the corrected volume flow, the automation system can continuously write different measured values to the measuring device:

- Medium temperature to increase the accuracy of the electrical conductivity (e.g. iTEMP)
- Reference density for calculating the corrected volume flow



Various pressure transmitters and temperature measuring devices can be ordered from Endress +Hauser: see "Accessories" section → 109

It is recommended to read in external measured values to calculate the following measured variables:  
Corrected volume flow

*HART protocol*

The measured values are written from the automation system to the measuring device via the HART protocol. The pressure transmitter must support the following protocol-specific functions:

- HART protocol
- Burst mode

*Current input*

The measured values are written from the automation system to the measuring device via the current input → 11.

*Digital communication*

The measured values can be written from the automation system to the measuring via:

- FOUNDATION Fieldbus
- PROFIBUS PA
- Modbus RS485
- EtherNet/IP
- PROFINET

**Current input 0/4 to 20 mA**

<b>Current input</b>	0/4 to 20 mA (active/passive)
<b>Current span</b>	<ul style="list-style-type: none"><li>■ 4 to 20 mA (active)</li><li>■ 0/4 to 20 mA (passive)</li></ul>
<b>Resolution</b>	1 µA
<b>Voltage drop</b>	Typically: 0.6 to 2 V for 3.6 to 22 mA (passive)
<b>Maximum input voltage</b>	≤ 30 V (passive)
<b>Open-circuit voltage</b>	≤ 28.8 V (active)
<b>Possible input variables</b>	<ul style="list-style-type: none"><li>■ Pressure</li><li>■ Temperature</li><li>■ Density</li></ul>

**Status input**

<b>Maximum input values</b>	<ul style="list-style-type: none"><li>■ DC -3 to 30 V</li><li>■ If status input is active (ON): <math>R_i &gt; 3 \text{ k}\Omega</math></li></ul>
<b>Response time</b>	Adjustable: 5 to 200 ms
<b>Input signal level</b>	<ul style="list-style-type: none"><li>■ Low signal: DC -3 to +5 V</li><li>■ High signal: DC 12 to 30 V</li></ul>
<b>Assignable functions</b>	<ul style="list-style-type: none"><li>■ Off</li><li>■ Reset the individual totalizers separately</li><li>■ Reset all totalizers</li><li>■ Flow override</li></ul>

## Output

### Output and input variants

Depending on the option selected for output/input 1, different options are available for the other outputs and inputs. Only one option can be selected for each output/input 1 to 3. The table must be read vertically (↓).

Example: If the option **BA** (current output 4 to 20 mA HART) was selected for output/input 1, one of the options **A, B, D, E, F, H, I** or **J** is available for output 2 and one of the options **A, B, D, E, F, H, I** or **J** is available for output 3.


Order code for "Output; input 1" (020) →	Possible options								
Current output 4 to 20 mA HART	<b>BA</b>								
Current output 4 to 20 mA HART Ex i	↓	<b>CA</b>							
FOUNDATION Fieldbus		↓	<b>SA</b>						
FOUNDATION Fieldbus Ex i			↓	<b>TA</b>					
PROFIBUS PA				↓	<b>GA</b>				
PROFIBUS PA Ex i					↓	<b>HA</b>			
Modbus RS485						↓	<b>MA</b>		
EtherNet/IP 2-port switch integrated							↓	<b>NA</b>	
PROFINET 2-port switch integrated								↓	<b>RA</b>
Order code for "Output; input 2" (021) →	↓	↓	↓	↓	↓	↓	↓	↓	↓
Not assigned	<b>A</b>	<b>A</b>	<b>A</b>	<b>A</b>	<b>A</b>	<b>A</b>	<b>A</b>	<b>A</b>	<b>A</b>
Current output 0/4 to 20 mA	<b>B</b>		<b>B</b>		<b>B</b>		<b>B</b>	<b>B</b>	<b>B</b>
Current output 0/4 to 20 mA (Ex i)		<b>C</b>		<b>C</b>		<b>C</b>			
User configurable input/output <sup>1)</sup>	<b>D</b>		<b>D</b>		<b>D</b>		<b>D</b>	<b>D</b>	<b>D</b>
Pulse/frequency/switch output	<b>E</b>		<b>E</b>		<b>E</b>		<b>E</b>	<b>E</b>	<b>E</b>
Double pulse output <sup>2)</sup>	<b>F</b>						<b>F</b>		
Pulse/frequency/switch output (Ex i)		<b>G</b>		<b>G</b>		<b>G</b>			
Relay output	<b>H</b>		<b>H</b>		<b>H</b>		<b>H</b>	<b>H</b>	<b>H</b>
Current input 0/4 to 20 mA	<b>I</b>		<b>I</b>		<b>I</b>		<b>I</b>	<b>I</b>	<b>I</b>
Status input	<b>J</b>		<b>J</b>		<b>J</b>		<b>J</b>	<b>J</b>	<b>J</b>
Order code for "Output; input 3" (022) →	↓	↓	↓	↓	↓	↓	↓	↓	↓
Not assigned	<b>A</b>	<b>A</b>	<b>A</b>	<b>A</b>	<b>A</b>	<b>A</b>	<b>A</b>	<b>A</b>	<b>A</b>
Current output 0/4 to 20 mA	<b>B</b>						<b>B</b>	<b>B</b>	<b>B</b>
Current output 0/4 to 20 mA (Ex i)		<b>C</b>							
User configurable input/output	<b>D</b>						<b>D</b>	<b>D</b>	<b>D</b>
Pulse/frequency/switch output	<b>E</b>						<b>E</b>	<b>E</b>	<b>E</b>
Double pulse output (slave)	<b>F</b>						<b>F</b>		
Pulse/frequency/switch output (Ex i)		<b>G</b>							
Relay output	<b>H</b>						<b>H</b>	<b>H</b>	<b>H</b>
Current input 0/4 to 20 mA	<b>I</b>						<b>I</b>	<b>I</b>	<b>I</b>
Status input	<b>J</b>						<b>J</b>	<b>J</b>	<b>J</b>

1) A specific input or output can be assigned to a user configurable input/output → 16.

2) If double pulse output (F) is selected for output/input 2 (021), only the double pulse output (F) option is available for selection for output/input 3 (022).



**Output signal****HART current output**

<b>Current output</b>	4 to 20 mA HART
<b>Current span</b>	Can be set to: 4 to 20 mA (active/passive)  Ex-i, passive
<b>Open-circuit voltage</b>	DC 28.8 V (active)
<b>Maximum input voltage</b>	DC 30 V (passive)
<b>Load</b>	250 to 700 $\Omega$
<b>Resolution</b>	0.38 $\mu$ A
<b>Damping</b>	Adjustable: 0.07 to 999 s
<b>Assignable measured variables</b>	<ul style="list-style-type: none"> <li>■ Volume flow</li> <li>■ Mass flow</li> <li>■ Corrected volume flow</li> <li>■ Flow velocity</li> <li>■ Conductivity</li> <li>■ Corrected conductivity</li> <li>■ Temperature</li> <li>■ Electronic temperature</li> </ul>

**PROFIBUS PA**

<b>PROFIBUS PA</b>	In accordance with EN 50170 Volume 2, IEC 61158-2 (MBP), galvanically isolated
<b>Data transfer</b>	31.25 kbit/s
<b>Current consumption</b>	10 mA
<b>Permitted supply voltage</b>	9 to 32 V
<b>Bus connection</b>	With integrated reverse polarity protection

**EtherNet/IP**

<b>Standards</b>	In accordance with IEEE 802.3
------------------	-------------------------------

**PROFINET**

<b>Standards</b>	In accordance with IEEE 802.3
------------------	-------------------------------


**FOUNDATION Fieldbus**

<b>FOUNDATION Fieldbus</b>	H1, IEC 61158-2, galvanically isolated
<b>Data transfer</b>	31.25 kbit/s
<b>Current consumption</b>	10 mA
<b>Permitted supply voltage</b>	9 to 32 V
<b>Bus connection</b>	With integrated reverse polarity protection


**Modbus RS485**

<b>Physical interface</b>	RS485 in accordance with EIA/TIA-485 standard
<b>Terminating resistor</b>	Integrated, can be activated via DIP switches

**Current output 0/4 to 20 mA**

<b>Current output</b>	0/4 to 20 mA
<b>Maximum output values</b>	22.5 mA
<b>Current span</b>	Can be set to: <ul style="list-style-type: none"> <li>■ 4 to 20 mA (active)</li> <li>■ 0/4 to 20 mA (passive)</li> </ul>  Ex-i, passive
<b>Open-circuit voltage</b>	DC 28.8 V (active)
<b>Maximum input voltage</b>	DC 30 V (passive)
<b>Load</b>	0 to 700 $\Omega$
<b>Resolution</b>	0.38 $\mu$ A
<b>Damping</b>	Adjustable: 0.07 to 999 s
<b>Assignable measured variables</b>	<ul style="list-style-type: none"> <li>■ Volume flow</li> <li>■ Mass flow</li> <li>■ Corrected volume flow</li> <li>■ Flow velocity</li> <li>■ Conductivity</li> <li>■ Corrected conductivity</li> <li>■ Temperature</li> <li>■ Electronic temperature</li> </ul>

**Pulse/frequency/switch output**

<b>Function</b>	Can be set to pulse, frequency or switch output
<b>Version</b>	Open collector Can be set to: <ul style="list-style-type: none"> <li>■ Active</li> <li>■ Passive</li> </ul>  Ex-i, passive
<b>Maximum input values</b>	DC 30 V, 250 mA (passive)
<b>Open-circuit voltage</b>	DC 28.8 V (active)
<b>Voltage drop</b>	For 22.5 mA: $\leq$ DC 2 V
<b>Pulse output</b>	
<b>Maximum input values</b>	DC 30 V, 250 mA (passive)
<b>Maximum output current</b>	22.5 mA (active)
<b>Open-circuit voltage</b>	DC 28.8 V (active)
<b>Pulse width</b>	Adjustable: 0.05 to 2 000 ms
<b>Maximum pulse rate</b>	10 000 Impulse/s
<b>Pulse value</b>	Adjustable
<b>Assignable measured variables</b>	<ul style="list-style-type: none"> <li>■ Volume flow</li> <li>■ Mass flow</li> <li>■ Corrected volume flow</li> </ul>
<b>Frequency output</b>	
<b>Maximum input values</b>	DC 30 V, 250 mA (passive)
<b>Maximum output current</b>	22.5 mA (active)
<b>Open-circuit voltage</b>	DC 28.8 V (active)
<b>Output frequency</b>	Adjustable: end value frequency 2 to 10 000 Hz ( $f_{\max} = 12\,500$ Hz)
<b>Damping</b>	Adjustable: 0 to 999 s

<b>Pulse/pause ratio</b>	1:1
<b>Assignable measured variables</b>	<ul style="list-style-type: none"> <li>■ Volume flow</li> <li>■ Mass flow</li> <li>■ Corrected volume flow</li> <li>■ Flow velocity</li> <li>■ Conductivity</li> <li>■ Corrected conductivity</li> <li>■ Temperature</li> <li>■ Electronic temperature</li> </ul>
<b>Switch output</b>	
<b>Maximum input values</b>	DC 30 V, 250 mA (passive)
<b>Open-circuit voltage</b>	DC 28.8 V (active)
<b>Switching behavior</b>	Binary, conductive or non-conductive
<b>Switching delay</b>	Adjustable: 0 to 100 s
<b>Number of switching cycles</b>	Unlimited
<b>Assignable functions</b>	<ul style="list-style-type: none"> <li>■ Off</li> <li>■ On</li> <li>■ Diagnostic behavior</li> <li>■ Limit value: <ul style="list-style-type: none"> <li>– Off</li> <li>– Volume flow</li> <li>– Mass flow</li> <li>– Corrected volume flow</li> <li>– Flow velocity</li> <li>– Conductivity</li> <li>– Corrected conductivity</li> <li>– Totalizer 1-3</li> <li>– Temperature</li> <li>– Electronic temperature</li> </ul> </li> <li>■ Flow direction monitoring</li> <li>■ Status <ul style="list-style-type: none"> <li>– Empty pipe detection</li> <li>– Low flow cut off</li> </ul> </li> </ul>

#### Double pulse output

<b>Function</b>	Double pulse
<b>Version</b>	Open collector Can be set to: <ul style="list-style-type: none"> <li>■ Active</li> <li>■ Passive</li> </ul>
<b>Maximum input values</b>	DC 30 V, 250 mA (passive)
<b>Open-circuit voltage</b>	DC 28.8 V (active)
<b>Voltage drop</b>	For 22.5 mA: ≤ DC 2 V
<b>Output frequency</b>	Adjustable: 0 to 1 000 Hz
<b>Damping</b>	Adjustable: 0 to 999 s
<b>Pulse/pause ratio</b>	1:1
<b>Assignable measured variables</b>	<ul style="list-style-type: none"> <li>■ Volume flow</li> <li>■ Mass flow</li> <li>■ Corrected volume flow</li> <li>■ Flow velocity</li> <li>■ Conductivity</li> <li>■ Corrected conductivity</li> <li>■ Temperature</li> <li>■ Electronic temperature</li> </ul>

**Relay output**

<b>Function</b>	Switch output
<b>Version</b>	Relay output, galvanically isolated
<b>Switching behavior</b>	Can be set to: <ul style="list-style-type: none"> <li>■ NO (normally open), factory setting</li> <li>■ NC (normally closed)</li> </ul>
<b>Maximum switching capacity (passive)</b>	<ul style="list-style-type: none"> <li>■ DC 30 V, 0.1 A</li> <li>■ AC 30 V, 0.5 A</li> </ul>
<b>Assignable functions</b>	<ul style="list-style-type: none"> <li>■ Off</li> <li>■ On</li> <li>■ Diagnostic behavior</li> <li>■ Limit value: <ul style="list-style-type: none"> <li>– Off</li> <li>– Volume flow</li> <li>– Mass flow</li> <li>– Corrected volume flow</li> <li>– Flow velocity</li> <li>– Conductivity</li> <li>– Corrected conductivity</li> <li>– Totalizer 1-3</li> <li>– Temperature</li> <li>– Electronic temperature</li> </ul> </li> <li>■ Flow direction monitoring</li> <li>■ Status <ul style="list-style-type: none"> <li>– Empty pipe detection</li> <li>– Low flow cut off</li> </ul> </li> </ul>

**User configurable input/output**

**One** specific input or output is assigned to a user-configurable input/output (configurable I/O) during device commissioning.

The following inputs and outputs are available for assignment:

- Choice of current output: 4 to 20 mA (active), 0/4 to 20 mA (passive)
- Pulse/frequency/switch output
- Choice of current input: 4 to 20 mA (active), 0/4 to 20 mA (passive)
- Status input

The technical values correspond to those of the inputs and outputs described in this section.

**Signal on alarm**

Depending on the interface, failure information is displayed as follows:

**HART current output**

<b>Device diagnostics</b>	Device condition can be read out via HART Command 48
---------------------------	--

**PROFIBUS PA**

<b>Status and alarm messages</b>	Diagnostics in accordance with PROFIBUS PA Profile 3.02
<b>Error current FDE (Fault Disconnection Electronic)</b>	0 mA

**EtherNet/IP**

<b>Device diagnostics</b>	Device condition can be read out in Input Assembly
---------------------------	--

**PROFINET**

<b>Device diagnostics</b>	According to "Application Layer protocol for decentralized periphery", Version 2.3
---------------------------	--

**FOUNDATION Fieldbus**

<b>Status and alarm messages</b>	Diagnostics in accordance with FF-891
<b>Error current FDE (Fault Disconnection Electronic)</b>	0 mA

**Modbus RS485**

<b>Failure mode</b>	Choose from: <ul style="list-style-type: none"> <li>■ NaN value instead of current value</li> <li>■ Last valid value</li> </ul>
---------------------	---

**Current output 0/4 to 20 mA***4 to 20 mA*

<b>Failure mode</b>	Choose from: <ul style="list-style-type: none"> <li>■ 4 to 20 mA in accordance with NAMUR recommendation NE 43</li> <li>■ 4 to 20 mA in accordance with US</li> <li>■ Min. value: 3.59 mA</li> <li>■ Max. value: 22.5 mA</li> <li>■ Freely definable value between: 3.59 to 22.5 mA</li> <li>■ Actual value</li> <li>■ Last valid value</li> </ul>
---------------------	--

*0 to 20 mA*

<b>Failure mode</b>	Choose from: <ul style="list-style-type: none"> <li>■ Maximum alarm: 22 mA</li> <li>■ Freely definable value between: 0 to 20.5 mA</li> </ul>
---------------------	---

**Pulse/frequency/switch output**

<b>Pulse output</b>	
<b>Failure mode</b>	Choose from: <ul style="list-style-type: none"> <li>■ Actual value</li> <li>■ No pulses</li> </ul>
<b>Frequency output</b>	
<b>Failure mode</b>	Choose from: <ul style="list-style-type: none"> <li>■ Actual value</li> <li>■ 0 Hz</li> <li>■ Defined value (<math>f_{\max}</math> 2 to 12 500 Hz)</li> </ul>
<b>Switch output</b>	
<b>Failure mode</b>	Choose from: <ul style="list-style-type: none"> <li>■ Current status</li> <li>■ Open</li> <li>■ Closed</li> </ul>

**Relay output**

<b>Failure mode</b>	Choose from: <ul style="list-style-type: none"> <li>■ Current status</li> <li>■ Open</li> <li>■ Closed</li> </ul>
---------------------	---

**Local display**

<b>Plain text display</b>	With information on cause and remedial measures
<b>Backlight</b>	Red backlighting indicates a device error.



Status signal as per NAMUR recommendation NE 107

**Interface/protocol**

- Via digital communication:
  - HART protocol
  - FOUNDATION Fieldbus
  - PROFIBUS PA
  - Modbus RS485
  - EtherNet/IP
  - PROFINET
- Via service interface
  - CDI-RJ45 service interface
  - WLAN interface

<b>Plain text display</b>	With information on cause and remedial measures
---------------------------	---



Additional information on remote operation → 92

**Web server**

<b>Plain text display</b>	With information on cause and remedial measures
---------------------------	---

**Light emitting diodes (LED)**

<b>Status information</b>	<p>Status indicated by various light emitting diodes</p> <p>The following information is displayed depending on the device version:</p> <ul style="list-style-type: none"> <li>■ Supply voltage active</li> <li>■ Data transmission active</li> <li>■ Device alarm/error has occurred</li> <li>■ EtherNet/IP network available</li> <li>■ EtherNet/IP connection established</li> <li>■ PROFINET network available</li> <li>■ PROFINET connection established</li> <li>■ PROFINET blinking feature</li> </ul>
---------------------------	---

## Ex connection data

## Safety-related values

Order code for "Output; input 1"	Output type	Safety-related values "Output; input 1"	
		26 (+)	27 (-)
Option <b>BA</b>	Current output 4 to 20 mA HART	$U_N = 30 \text{ V}_{DC}$ $U_M = 250 \text{ V}_{AC}$	
Option <b>GA</b>	PROFIBUS PA	$U_N = 30 \text{ V}_{DC}$ $U_M = 250 \text{ V}_{AC}$	
Option <b>MA</b>	Modbus RS485	$U_N = 30 \text{ V}_{DC}$ $U_M = 250 \text{ V}_{AC}$	
Option <b>SA</b>	FOUNDATION Fieldbus	$U_N = 30 \text{ V}_{DC}$ $U_M = 250 \text{ V}_{AC}$	
Option <b>NA</b>	EtherNet/IP	$U_N = 30 \text{ V}_{DC}$ $U_M = 250 \text{ V}_{AC}$	
Option <b>RA</b>	PROFINET	$U_N = 30 \text{ V}_{DC}$ $U_M = 250 \text{ V}_{AC}$	

Order code for "Output; input 2"; "Output; input 3"	Output type	Safety-related values			
		Output; input 2		Output; input 3	
		24 (+)	25 (-)	22 (+)	23 (-)
Option <b>B</b>	Current output 4 to 20 mA	$U_N = 30 \text{ V}_{DC}$ $U_M = 250 \text{ V}_{AC}$			
Option <b>D</b>	User configurable input/ output	$U_N = 30 \text{ V}_{DC}$ $U_M = 250 \text{ V}_{AC}$			
Option <b>E</b>	Pulse/frequency/switch output	$U_N = 30 \text{ V}_{DC}$ $U_M = 250 \text{ V}_{AC}$			
Option <b>F</b>	Double pulse output	$U_N = 30 \text{ V}_{DC}$ $U_M = 250 \text{ V}_{AC}$			
Option <b>H</b>	Relay output	$U_N = 30 \text{ V}_{DC}$ $I_N = 100 \text{ mA}_{DC}/500 \text{ mA}_{AC}$ $U_M = 250 \text{ V}_{AC}$			
Option <b>I</b>	Current input 4 to 20 mA	$U_N = 30 \text{ V}_{DC}$ $U_M = 250 \text{ V}_{AC}$			
Option <b>J</b>	Status input	$U_N = 30 \text{ V}_{DC}$ $U_M = 250 \text{ V}_{AC}$			

## Intrinsically safe values

Order code for "Output; input 1"	Output type	Intrinsically safe values "Output; input 1"	
		26 (+)	27 (-)
Option <b>CA</b>	Current output 4 to 20 mA HART Ex i	$U_i = 30\text{ V}$ $I_i = 100\text{ mA}$ $P_i = 1.25\text{ W}$ $L_i = 0$ $C_i = 0$	
Option <b>HA</b>	PROFIBUS PA Ex i	<b>Ex ia</b> <sup>1)</sup> $U_i = 30\text{ V}$ $I_i = 570\text{ mA}$ $P_i = 8.5\text{ W}$ $L_i = 10\text{ }\mu\text{H}$ $C_i = 5\text{ nF}$	<b>Ex ic</b> <sup>2)</sup> $U_i = 32\text{ V}$ $I_i = 570\text{ mA}$ $P_i = 8.5\text{ W}$ $L_i = 10\text{ }\mu\text{H}$ $C_i = 5\text{ nF}$
Option <b>TA</b>	FOUNDATION Fieldbus Ex i	<b>Ex ia</b> $U_i = 30\text{ V}$ $I_i = 570\text{ mA}$ $P_i = 8.5\text{ W}$ $L_i = 10\text{ }\mu\text{H}$ $C_i = 5\text{ nF}$	<b>Ex ic</b> $U_i = 32\text{ V}$ $I_i = 570\text{ mA}$ $P_i = 8.5\text{ W}$ $L_i = 10\text{ }\mu\text{H}$ $C_i = 5\text{ nF}$

1) Only available for the Zone 1, Class I, Division 1 version

2) Only available for the Zone 2, Class I, Division 2 version transmitter

Order code for "Output; input 2"; "Output; input 3"	Output type	Intrinsically safe values or NIFW values			
		Output; input 2		Output; input 3	
		24 (+)	25 (-)	22 (+)	23 (-)
Option <b>C</b>	Current output 4 to 20 mA Ex i	$U_i = 30\text{ V}$ $I_i = 100\text{ mA}$ $P_i = 1.25\text{ W}$ $L_i = 0$ $C_i = 0$			
Option <b>G</b>	Pulse/frequency/switch output Ex i	$U_i = 30\text{ V}$ $I_i = 100\text{ mA}$ $P_i = 1.25\text{ W}$ $L_i = 0$ $C_i = 0$			

## Low flow cut off

The switch points for low flow cut off are user-selectable.

## Galvanic isolation

The outputs are galvanically isolated from one another and from earth (PE).




## Protocol-specific data

## HART

Manufacturer ID	0x11
Device type ID	0x3C
HART protocol revision	7
Device description files (DTM, DD)	Information and files under: <a href="http://www.endress.com">www.endress.com</a>
HART load	Min. 250 $\Omega$
System integration	Information on system integration: Operating Instructions → 109. <ul style="list-style-type: none"> <li>Measured variables via HART protocol</li> <li>Burst Mode functionality</li> </ul>



## PROFIBUS PA

<b>Manufacturer ID</b>	0x11
<b>Ident number</b>	0x156C
<b>Profile version</b>	3.02
<b>Device description files (GSD, DTM, DD)</b>	Information and files under: <ul style="list-style-type: none"> <li>▪ <a href="http://www.endress.com">www.endress.com</a></li> <li>▪ <a href="http://www.profibus.org">www.profibus.org</a></li> </ul>
<b>Supported functions</b>	<ul style="list-style-type: none"> <li>▪ Identification &amp; Maintenance Simplest device identification on the part of the control system and nameplate</li> <li>▪ PROFIBUS upload/download Reading and writing parameters is up to ten times faster with PROFIBUS upload/download</li> <li>▪ Condensed status Simplest and self-explanatory diagnostic information by categorizing diagnostic messages that occur</li> </ul>
<b>Configuration of the device address</b>	<ul style="list-style-type: none"> <li>▪ DIP switches on the I/O electronics module</li> <li>▪ Local display</li> <li>▪ Via operating tools (e.g. FieldCare)</li> </ul>
<b>Compatibility with earlier model</b>	<p>If the device is replaced, the measuring device Promag 300 supports the compatibility of the cyclic data with previous models. It is not necessary to adjust the engineering parameters of the PROFIBUS network with the Promag 300 GSD file.</p> <p>Earlier models:</p> <ul style="list-style-type: none"> <li>▪ Promag 50 PROFIBUS PA <ul style="list-style-type: none"> <li>– ID No.: 1525 (hex)</li> <li>– Extended GSD file: EH3x1525.gsd</li> <li>– Standard GSD file: EH3_1525.gsd</li> </ul> </li> <li>▪ Promag 53 PROFIBUS PA <ul style="list-style-type: none"> <li>– ID No.: 1527 (hex)</li> <li>– Extended GSD file: EH3x1527.gsd</li> <li>– Standard GSD file: EH3_1527.gsd</li> </ul> </li> </ul> <p> Description of the function scope of compatibility: Operating Instructions →  109.</p>
<b>System integration</b>	<p>Information regarding system integration: Operating Instructions →  109.</p> <ul style="list-style-type: none"> <li>▪ Cyclic data transmission</li> <li>▪ Block model</li> <li>▪ Description of the modules</li> </ul>


## EtherNet/IP

<b>Protocol</b>	<ul style="list-style-type: none"> <li>▪ The CIP Networks Library Volume 1: Common Industrial Protocol</li> <li>▪ The CIP Networks Library Volume 2: EtherNet/IP Adaptation of CIP</li> </ul>
<b>Communication type</b>	<ul style="list-style-type: none"> <li>▪ 10Base-T</li> <li>▪ 100Base-TX</li> </ul>
<b>Device profile</b>	Generic device (product type: 0x2B)
<b>Manufacturer ID</b>	0x11
<b>Device type ID</b>	0x103C
<b>Baud rates</b>	Automatic $10^{100}$ Mbit with half-duplex and full-duplex detection
<b>Polarity</b>	Auto-polarity for automatic correction of crossed Tx/D and Rx/D pairs
<b>Supported CIP connections</b>	Max. 3 connections
<b>Explicit connections</b>	Max. 6 connections
<b>I/O connections</b>	Max. 6 connections (scanner)

<b>Configuration options for measuring device</b>	<ul style="list-style-type: none"> <li>▪ DIP switches on the electronics module for IP addressing</li> <li>▪ Manufacturer-specific software (FieldCare)</li> <li>▪ Add-on Profile Level 3 for Rockwell Automation control systems</li> <li>▪ Web browser</li> <li>▪ Electronic Data Sheet (EDS) integrated in the measuring device</li> </ul>
<b>Configuration of the EtherNet interface</b>	<ul style="list-style-type: none"> <li>▪ Speed: 10 MBit, 100 MBit, auto (factory setting)</li> <li>▪ Duplex: half-duplex, full-duplex, auto (factory setting)</li> </ul>
<b>Configuration of the device address</b>	<ul style="list-style-type: none"> <li>▪ DIP switches on the electronics module for IP addressing (last octet)</li> <li>▪ DHCP</li> <li>▪ Manufacturer-specific software (FieldCare)</li> <li>▪ Add-on Profile Level 3 for Rockwell Automation control systems</li> <li>▪ Web browser</li> <li>▪ EtherNet/IP tools, e.g. RSLinx (Rockwell Automation)</li> </ul>
<b>Device Level Ring (DLR)</b>	Yes
<b>System integration</b>	<p>Information regarding system integration: Operating Instructions → 109.</p> <ul style="list-style-type: none"> <li>▪ Cyclic data transmission</li> <li>▪ Block model</li> <li>▪ Input and output groups</li> </ul>


## PROFINET

<b>Protocol</b>	"Application layer protocol for decentral device periphery and distributed automation", version 2.3
<b>Communication type</b>	100 MBit/s
<b>Conformity class</b>	Conformance Class B
<b>Netload Class</b>	Netload Class II
<b>Baud rates</b>	Automatic 100 Mbit/s with full-duplex detection
<b>Cycle times</b>	From 8 ms
<b>Polarity</b>	Auto-polarity for automatic correction of crossed TxD and RxD pairs
<b>Media Redundancy Protocol (MRP)</b>	Yes
<b>Device profile</b>	Application interface identifier 0xF600 Generic device
<b>Manufacturer ID</b>	0x11
<b>Device type ID</b>	0x843C
<b>Device description files (GSD, DTM, DD)</b>	<p>Information and files under:</p> <ul style="list-style-type: none"> <li>▪ <a href="http://www.endress.com">www.endress.com</a> On the product page for the device: Documents/Software → Device drivers</li> <li>▪ <a href="http://www.profibus.org">www.profibus.org</a></li> </ul>
<b>Supported connections</b>	<ul style="list-style-type: none"> <li>▪ 1 x AR (IO Controller AR)</li> <li>▪ 1 x AR (IO-Supervisor Device AR connection allowed)</li> <li>▪ 1 x Input CR (Communication Relation)</li> <li>▪ 1 x Output CR (Communication Relation)</li> <li>▪ 1 x Alarm CR (Communication Relation)</li> </ul>
<b>Configuration options for measuring device</b>	<ul style="list-style-type: none"> <li>▪ DIP switches on the electronics module, for device name assignment (last part)</li> <li>▪ Manufacturer-specific software (FieldCare, DeviceCare)</li> <li>▪ Web browser</li> <li>▪ Device master file (GSD), can be read out via the integrated Web server of the measuring device</li> </ul>
<b>Configuration of the device name</b>	<ul style="list-style-type: none"> <li>▪ DIP switches on the electronics module, for device name assignment (last part)</li> <li>▪ DCP protocol</li> <li>▪ Process Device Manager (PDM)</li> <li>▪ Integrated Web server</li> </ul>





<b>Supported functions</b>	<ul style="list-style-type: none"> <li>■ Identification &amp; Maintenance Simple device identification via: <ul style="list-style-type: none"> <li>– Control system</li> <li>– Nameplate</li> </ul> </li> <li>■ Measured value status The process variables are communicated with a measured value status</li> <li>■ Blinking feature via the onsite display for simple device identification and assignment</li> <li>■ Device operation via operating tools (e.g. FieldCare, DeviceCare, SIMATIC PDM)</li> </ul>
<b>System integration</b>	<p>Information regarding system integration: Operating Instructions →  109.</p> <ul style="list-style-type: none"> <li>■ Cyclic data transmission</li> <li>■ Overview and description of the modules</li> <li>■ Status coding</li> <li>■ Startup configuration</li> <li>■ Factory setting:</li> </ul>

### FOUNDATION Fieldbus

<b>Manufacturer ID</b>	0x452B48 (hex)
<b>Ident number</b>	0x103C (hex)
<b>Device revision</b>	1
<b>DD revision</b>	Information and files under:
<b>CFF revision</b>	<ul style="list-style-type: none"> <li>■ <a href="http://www.endress.com">www.endress.com</a></li> <li>■ <a href="http://www.fieldbus.org">www.fieldbus.org</a></li> </ul>
<b>Interoperability Test Kit (ITK)</b>	Version 6.2.0
<b>ITK Test Campaign Number</b>	Information: <ul style="list-style-type: none"> <li>■ <a href="http://www.endress.com">www.endress.com</a></li> <li>■ <a href="http://www.fieldbus.org">www.fieldbus.org</a></li> </ul>
<b>Link Master capability (LAS)</b>	Yes
<b>Choice of "Link Master" and "Basic Device"</b>	Yes Factory setting: Basic Device
<b>Node address</b>	Factory setting: 247 (0xF7)
<b>Supported functions</b>	<p>The following methods are supported:</p> <ul style="list-style-type: none"> <li>■ Restart</li> <li>■ ENP Restart</li> <li>■ Diagnostic</li> <li>■ Set to OOS</li> <li>■ Set to AUTO</li> <li>■ Read trend data</li> <li>■ Read event logbook</li> </ul>
<b>Virtual Communication Relationships (VCRs)</b>	
<b>Number of VCRs</b>	44
<b>Number of link objects in VFD</b>	50
<b>Permanent entries</b>	1
<b>Client VCRs</b>	0
<b>Server VCRs</b>	10
<b>Source VCRs</b>	43
<b>Sink VCRs</b>	0
<b>Subscriber VCRs</b>	43
<b>Publisher VCRs</b>	43
<b>Device Link Capabilities</b>	
<b>Slot time</b>	4
<b>Min. delay between PDU</b>	8

<b>Max. response delay</b>	16
<b>System integration</b>	Information regarding system integration: Operating Instructions →  109. <ul style="list-style-type: none"> <li>▪ Cyclic data transmission</li> <li>▪ Description of the modules</li> <li>▪ Execution times</li> <li>▪ Methods</li> </ul>

### Modbus RS485

<b>Protocol</b>	Modbus Applications Protocol Specification V1.1
<b>Response times</b>	<ul style="list-style-type: none"> <li>▪ Direct data access: typically 25 to 50 ms</li> <li>▪ Auto-scan buffer (data range): typically 3 to 5 ms</li> </ul>
<b>Device type</b>	Slave
<b>Slave address range</b>	1 to 247
<b>Broadcast address range</b>	0
<b>Function codes</b>	<ul style="list-style-type: none"> <li>▪ 03: Read holding register</li> <li>▪ 04: Read input register</li> <li>▪ 06: Write single registers</li> <li>▪ 08: Diagnostics</li> <li>▪ 16: Write multiple registers</li> <li>▪ 23: Read/write multiple registers</li> </ul>
<b>Broadcast messages</b>	Supported by the following function codes: <ul style="list-style-type: none"> <li>▪ 06: Write single registers</li> <li>▪ 16: Write multiple registers</li> <li>▪ 23: Read/write multiple registers</li> </ul>
<b>Supported baud rate</b>	<ul style="list-style-type: none"> <li>▪ 1 200 BAUD</li> <li>▪ 2 400 BAUD</li> <li>▪ 4 800 BAUD</li> <li>▪ 9 600 BAUD</li> <li>▪ 19 200 BAUD</li> <li>▪ 38 400 BAUD</li> <li>▪ 57 600 BAUD</li> <li>▪ 115 200 BAUD</li> </ul>
<b>Data transfer mode</b>	<ul style="list-style-type: none"> <li>▪ ASCII</li> <li>▪ RTU</li> </ul>
<b>Data access</b>	Each device parameter can be accessed via Modbus RS485.  For Modbus register information
<b>Compatibility with earlier model</b>	If the device is replaced, the measuring device Promag 300 supports the compatibility of the Modbus registers for the process variables and the diagnostic information with previous models Promag 53. It is not necessary to change the engineering parameters in the automation system.  Description of the function scope of compatibility: Operating Instructions →  109.
<b>System integration</b>	Information on system integration: Operating Instructions →  109. <ul style="list-style-type: none"> <li>▪ Modbus RS485 information</li> <li>▪ Function codes</li> <li>▪ Register information</li> <li>▪ Response time</li> <li>▪ Modbus data map</li> </ul>

## Power supply

### Terminal assignment

#### Transmitter: supply voltage, input/outputs

##### HART

Supply voltage		Input/output 1		Input/output 2		Input/output 3	
1 (+)	2 (-)	26 (+)	27 (-)	24 (+)	25 (-)	22 (+)	23 (-)
The terminal assignment depends on the specific device version ordered → 12.							

##### FOUNDATION Fieldbus

Supply voltage		Input/output 1		Input/output 2		Input/output 3	
1 (+)	2 (-)	26 (A)	27 (B)	24 (+)	25 (-)	22 (+)	23 (-)
The terminal assignment depends on the specific device version ordered → 12.							


##### PROFIBUS PA

Supply voltage		Input/output 1		Input/output 2		Input/output 3	
1 (+)	2 (-)	26 (B)	27 (A)	24 (+)	25 (-)	22 (+)	23 (-)
The terminal assignment depends on the specific device version ordered → 12.							


##### Modbus RS485

Supply voltage		Input/output 1		Input/output 2		Input/output 3	
1 (+)	2 (-)	26 (B)	27 (A)	24 (+)	25 (-)	22 (+)	23 (-)
The terminal assignment depends on the specific device version ordered → 12.							

##### PROFINET

Supply voltage		Input/output 1	Input/output 2		Input/output 3	
1 (+)	2 (-)	PROFINET (RJ45 connector)	24 (+)	25 (-)	22 (+)	23 (-)
The terminal assignment depends on the specific device version ordered →  12.						

##### EtherNet/IP

Supply voltage		Input/output 1	Input/output 2		Input/output 3	
1 (+)	2 (-)	EtherNet/IP (RJ45 connector)	24 (+)	25 (-)	22 (+)	23 (-)
The terminal assignment depends on the specific device version ordered →  12.						



Terminal assignment of the remote display and operating module → 30.

### Device plugs available



Device plugs may not be used in hazardous areas!

#### Device plugs for fieldbus systems:

Order code for "Input; output 1"

- Option **SA** "FOUNDATION Fieldbus" → 26
- Option **GA** "PROFIBUS PA" → 26
- Option **RA** "PROFINET" → 26
- Option **NA** "EtherNet/IP" → 26

**Device plug for connecting to the service interface:**

Order code for "Accessory mounted"

option **NB**, adapter RJ45 M12 (service interface) → 27**Order code for "Input; output 1", option SA "FOUNDATION Fieldbus"**

Order code for "Electrical connection"	Cable entry/connection → 29	
	2	3
M, 3, 4, 5	7/8" connector	–

**Order code for "Input; output 1", option GA "PROFIBUS PA"**

Order code for "Electrical connection"	Cable entry/connection → 29	
	2	3
L, N, P, U	Connector M12 × 1	–

**Order code for "Input; output 1", option RA "PROFINET"**

Order code for "Electrical connection"	Cable entry/connection → 29	
	2	3
L, N, P, U	Connector M12 × 1	–
R <sup>1) 2)</sup> , S <sup>1) 2)</sup> , T <sup>1) 2)</sup> , V <sup>1) 2)</sup>	Connector M12 × 1	Connector M12 × 1

- 1) Cannot be combined with an external WLAN antenna (order code for "Enclosed accessories", option P8) of an RJ45 M12 adapter for the service interface (order code for "Accessories mounted", option NB) or of the remote display and operating module DKX001.
- 2) Suitable for integrating the device in a ring topology.

**Order code for "Input; output 1", option NA "EtherNet/IP"**


Order code for "Electrical connection"	Cable entry/connection → 29	
	2	3
L, N, P, U	Connector M12 × 1	–
R <sup>1) 2)</sup> , S <sup>1) 2)</sup> , T <sup>1) 2)</sup> , V <sup>1) 2)</sup>	Connector M12 × 1	Connector M12 × 1

- 1) Cannot be combined with an external WLAN antenna (order code for "Enclosed accessories", option P8) of an RJ45 M12 adapter for the service interface (order code for "Accessories mounted", option NB) or of the remote display and operating module DKX001.
- 2) Suitable for integrating the device in a ring topology.

**Order code for "Accessory mounted", option NB "Adapter RJ45 M12 (service interface)"**


Order code "Accessory mounted"	Cable entry/coupling → 29	
	Cable entry 2	Cable entry 3
NB	Plug M12 × 1	–

**Pin assignment, device plug****FOUNDATION Fieldbus**


	Pin	Assignment		Coding	Plug/socket
	1	+	Signal +	A	Plug
	2	-	Signal -		

	3		Grounding		
	4		Not assigned		

PROFIBUS PA

	Pin	Assignment		Coding	Plug/socket
	1	+	PROFIBUS PA +	A	Plug
	2		Grounding		
	3	-	PROFIBUS PA -		
	4		Not assigned		


PROFINET

 A0016812	Pin	Assignment	
	1	+	TD +
	2	+	RD +
	3	-	TD -
	4	-	RD -
	Coding		Plug/socket
	D		Socket



- Recommended plug:
- Binder, series 763, part no. 99 3729 810 04
  - Phoenix, part no. 1543223 SACC-M12MSD-4Q
  - When using the device in a hazardous location, use a suitably certified plug.

EtherNet/IP


 A0016812	Pin	Assignment	
	1	+	Tx
	2	+	Rx
	3	-	Tx
	4	-	Rx
	Coding		Plug/socket
	D		Socket



- Recommended plug:
- Binder, series 763, part no. 99 3729 810 04
  - Phoenix, part no. 1543223 SACC-M12MSD-4Q
  - When using the device in a hazardous location, use a suitably certified plug.

Service interface

Order code for "Accessories mounted", option **NB**: Adapter RJ45 M12 (service interface)

 A0016812	Pin	Assignment	
	1	+	Tx
	2	+	Rx
	3	-	Tx
	4	-	Rx
	Coding		Plug/socket
	D		Socket



Recommended plug:

- Binder, series 763, part no. 99 3729 810 04
- Phoenix, part no. 1543223 SACC-M12MSD-4Q
- When using the device in a hazardous location, use a suitably certified plug.

Supply voltage	Order code for "Power supply"	terminal voltage		Frequency range
	Option D	DC24 V	±20%	–
	Option E	AC100 to 240 V	–15...+10%	50/60 Hz, ±4 Hz
	Option I	DC24 V	±20%	–
		AC100 to 240 V	–15...+10%	50/60 Hz, ±4 Hz

**Power consumption**      **Transmitter**  
Max. 10 W (active power)

**Current consumption**      **Transmitter**

- Max. 400 mA (24 V)
- Max. 200 mA (110 V, 50/60 Hz; 230 V, 50/60 Hz)

**Power supply failure**

- Totalizers stop at the last value measured.
- Configuration is retained in the plug-in memory (HistoROM DAT).
- Error messages (incl. total operated hours) are stored.




## Electrical connection

## Connecting the transmitter



- Terminal assignment → 25
- Device plugs available → 25



A0026781

- 1 Terminal connection for supply voltage
- 2 Terminal connection for signal transmission, input/output
- 3 Terminal connection for signal transmission, input/output or terminal for network connection via service interface (CDI-RJ45); Optional: terminal connection for external WLAN antenna or connection for remote display and operating module DKX001
- 4 Protective ground (PE)



An adapter for RJ45 and the M12 connector is optionally available:  
Order code for "Accessories", option **NB**: "Adapter RJ45 M12 (service interface)"

The adapter connects the service interface (CDI-RJ45) to an M12 connector mounted in the cable entry. Therefore the connection to the service interface can be established via an M12 connector without opening the device.



Network connection via service interface (CDI-RJ45) → 97


## Connecting in a ring topology

Device versions with EtherNet/IP and PROFINET communication protocols can be integrated into a ring topology. The device is integrated via the terminal connection for signal transmission (output 1) and the connection to the service interface (CDI-RJ45).



Integrate the transmitter into a ring topology:

- EtherNet/IP → 95
- PROFINET → 96



A0026781


- 1 Terminal connection for supply voltage
- 2 Terminal connection for signal transmission: PROFINET or EtherNet/IP (RJ45 connector)
- 3 Connection to service interface (CDI-RJ45)
- 4 Protective earth (PE)



If the device has additional input/outputs, these are routed via the cable entry for the connection to the service interface (CDI-RJ45).

### Connecting the remote display and operating module DKX001

- i** The remote display and operating module DKX001 is available as an optional extra → 106.
- The remote display and operating module DKX001 is only available for the following housing version: order code for "Housing": option A "Aluminum, coated"
  - The measuring device is always supplied with a dummy cover when the remote display and operating module DKX001 is ordered directly with the measuring device. Display or operation at the transmitter is not possible in this case.
  - If ordered subsequently, the remote display and operating module DKX001 may not be connected at the same time as the existing measuring device display module. Only one display or operation unit may be connected to the transmitter at any one time.




A0027518

- 1 Remote display and operating module DKX001
- 2 Protective earth (PE)
- 3 Connecting cable
- 4 Measuring device
- 5 Protective earth (PE)


### Connection examples

#### Current output 4 to 20 mA HART



A0029055

- 2** Connection example for 4 to 20 mA HART current output (active)
- 1 Automation system with current input (e.g. PLC)
  - 2 Cable shield: the cable shield must be grounded at both ends to comply with EMC requirements; observe cable specifications → 39
  - 3 Connection for HART operating devices → 92
  - 4 Resistor for HART communication ( $\geq 250 \Omega$ ): observe maximum load → 13
  - 5 Analog display unit: observe maximum load → 13
  - 6 Transmitter




A0028762

3 Connection example for 4 to 20 mA HART current output (passive)

- 1 Automation system with current input (e.g. PLC)
- 2 Power supply
- 3 Cable shield: the cable shield must be grounded at both ends to comply with EMC requirements; observe cable specifications → 39
- 4 Analog display unit: observe maximum load → 13
- 5 Transmitter

### HART input




A0028763

4 Connection example for HART input with a common negative (passive)

- 1 Automation system with HART output (e.g. PLC)
- 2 Active barrier for power supply (e.g. RN221N)
- 3 Cable shield: the cable shield must be grounded at both ends to comply with EMC requirements; observe cable specifications
- 4 Analog display unit: observe maximum load
- 5 Pressure transmitter (e.g. Cerabar M, Cerabar S): see requirements
- 6 Transmitter

## PROFIBUS-PA




A0028768

5 Connection example for PROFIBUS-PA

- 1 Control system (e.g. PLC)
- 2 PROFIBUS PA segment coupler
- 3 Cable shield: the cable shield must be grounded at both ends to comply with EMC requirements; observe cable specifications
- 4 T-box
- 5 Measuring device
- 6 Local grounding
- 7 Bus terminator
- 8 Potential matching line

## EtherNet/IP

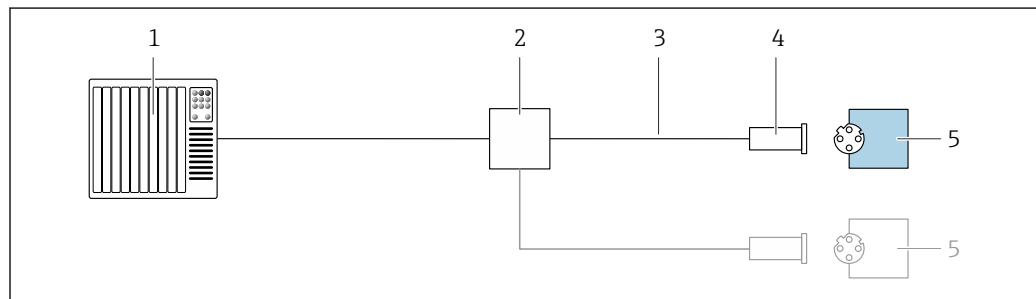


A0028767

6 Connection example for EtherNet/IP


- 1 Control system (e.g. PLC)
- 2 Ethernet switch
- 3 Observe cable specifications
- 4 Device plug
- 5 Transmitter

### EtherNet/IP: DLR (Device Level Ring)



- 1 Control system (e.g. PLC)
- 2 Ethernet switch
- 3 Observe cable specifications → 39
- 4 Connecting cable between the two transmitters
- 5 Transmitter


### PROFINET

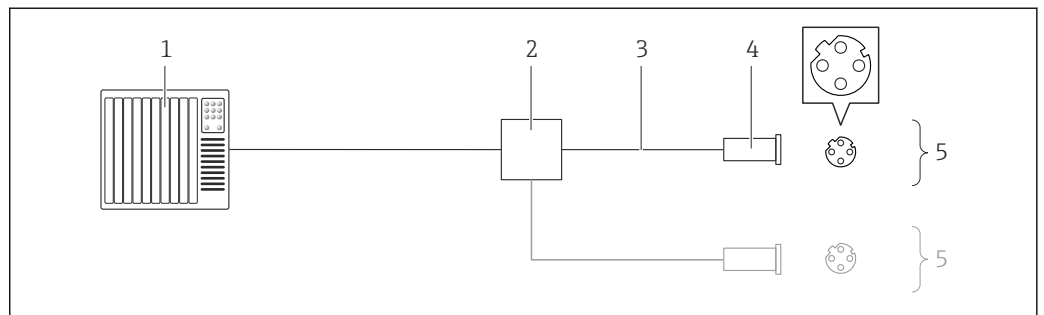

#### 7 Connection example for PROFINET


- 1 Control system (e.g. PLC)
- 2 Ethernet switch
- 3 Observe cable specifications
- 4 Device plug
- 5 Transmitter

### PROFINET: MRP (Media Redundancy Protocol)



- 1 Control system (e.g. PLC)
- 2 Ethernet switch
- 3 Observe cable specifications → 39
- 4 Connecting cable between the two transmitters
- 5 Transmitter

## FOUNDATION Fieldbus

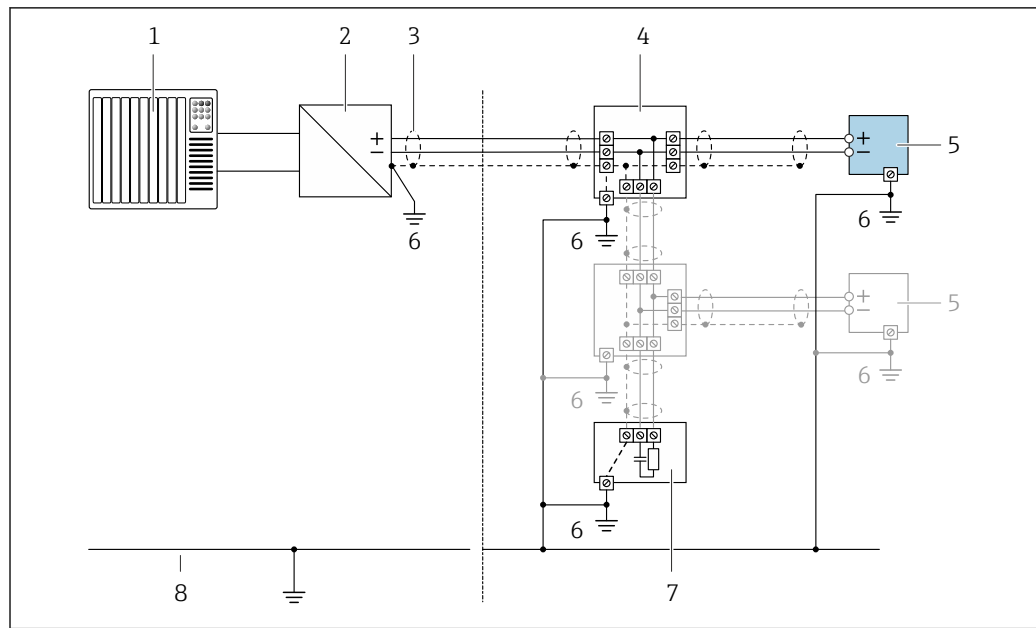


A0028768

8 Connection example for FOUNDATION Fieldbus

- 1 Control system (e.g. PLC)
- 2 Power Conditioner (FOUNDATION Fieldbus)
- 3 Cable shield: the cable shield must be grounded at both ends to comply with EMC requirements; observe cable specifications
- 4 T-box
- 5 Measuring device
- 6 Local grounding
- 7 Bus terminator
- 8 Potential matching line

## Modbus RS485




A0028765

9 Connection example for Modbus RS485, non-hazardous area and Zone 2/Div. 2

- 1 Control system (e.g. PLC)
- 2 Cable shield: the cable shield must be grounded at both ends to comply with EMC requirements; observe cable specifications
- 3 Distribution box
- 4 Transmitter


### Current output 4-20 mA



A0028758

10 Connection example for 4-20 mA current output (active)

- 1 Automation system with current input (e.g. PLC)
- 2 Analog display unit: observe maximum load
- 3 Transmitter




A0028759

11 Connection example for 4-20 mA current output (passive)

- 1 Automation system with current input (e.g. PLC)
- 2 Active barrier for power supply (e.g. RN221N)
- 3 Analog display unit: observe maximum load
- 4 Transmitter

### Pulse/frequency output



A0028761

12 Connection example for pulse/frequency output (passive)


- 1 Automation system with pulse/frequency input (e.g. PLC)
- 2 Power supply
- 3 Transmitter: Observe input values → 14

## Endress+Hauser




A0029280

A0029279

- 1 Automation system with double pulse input (e.g. PLC)
- 2 Power supply
- 3 Transmitter: Observe input values →  15
- 4 Double pulse output
- 5 Double pulse output (slave), phase-shifted



### Relay output




A0028760

16 Connection example for relay output (passive)

- 1 Automation system with relay input (e.g. PLC)
- 2 Power supply
- 3 Transmitter: Observe input values → 16

### Current input




A0028915

17 Connection example for 4 to 20 mA current input

- 1 Power supply
- 2 External measuring device (for reading in pressure or temperature, for instance)
- 3 Transmitter: Observe input values

### Status input



A0028764

18 Connection example for status input

- 1 Automation system with status output (e.g. PLC)
- 2 Power supply
- 3 Transmitter: Observe input values

### Potential equalization

### Requirements

Please consider the following to ensure correct measurement:

- Same electrical potential for the medium and sensor
- Company-internal grounding concepts
- Pipe material and grounding

## Connection example, standard scenario

### *Metal process connections*

Potential equalization is generally via the metal process connections that are in contact with the medium and mounted directly on the sensor. Therefore there is generally no need for additional potential equalization measures.

## Connection example in special situations


### *Plastic process connections*

In the case of plastic process connections, additional grounding rings or process connections with an integrated grounding electrode must be used to ensure potential matching between the sensor and the fluid. If there is no potential matching, this can affect the measuring accuracy or cause the destruction of the sensor as a result of the electrochemical decomposition of the electrodes.

Note the following when using grounding rings:

- Depending on the option ordered, plastic disks are used instead of grounding rings on some process connections. These plastic disks only act as "spacers" and do not have any potential matching function. Furthermore, they also perform a significant sealing function at the sensor/ connection interface. Therefore, in the case of process connections without metal grounding rings, these plastic disks/seals should never be removed and should always be installed!
- Grounding rings can be ordered separately as an accessory from Endress+Hauser. When ordering make sure that the grounding rings are compatible with the material used for the electrodes, as otherwise there is the danger that the electrodes could be destroyed by electrochemical corrosion!
- Grounding rings, including seals, are mounted inside the process connections. Therefore the installation length is not affected.


### *Potential equalization via additional grounding ring*



A0028971

- 1 Hexagonal-headed bolts of process connection
- 2 O-ring seals
- 3 Plastic disk (spacer) or grounding ring
- 4 Sensor

Potential equalization via grounding electrodes on process connection



A0028972

- 1 Hexagonal-headed bolts of process connection
- 2 Integrated grounding electrodes
- 3 O-ring seal
- 4 Sensor

#### terminals

Spring-loaded terminals: Suitable for strands and strands with ferrules.  
Conductor cross-section 0.2 to 2.5 mm<sup>2</sup> (24 to 12 AWG).

#### Cable entries

- Cable gland: M20 × 1.5 with cable Ø 6 to 12 mm (0.24 to 0.47 in)
- Thread for cable entry:
  - NPT ½"
  - G ½"
  - M20
- Device plug for digital communication: M12  
Only available for certain device versions → 25.

#### Cable specification

##### Permitted temperature range

- The installation guidelines that apply in the country of installation must be observed.
- The cables must be suitable for the minimum and maximum temperatures to be expected.

##### Power supply cable

Standard installation cable is sufficient.

##### Signal cable

Current output 4 to 20 mA HART

A shielded cable is recommended. Observe grounding concept of the plant.

##### PROFIBUS PA

Twisted, shielded two-wire cable. Cable type A is recommended .



For further information on planning and installing PROFIBUS PA networks see:

- Operating Instructions "PROFIBUS DP/PA: Guidelines for planning and commissioning" (BA00034S)
- PNO Directive 2.092 "PROFIBUS PA User and Installation Guideline"
- IEC 61158-2 (MBP)

##### EtherNet/IP

The standard ANSI/TIA/EIA-568-B.2 Annex specifies CAT 5 as the minimum category for a cable used for EtherNet/IP. CAT 5e and CAT 6 are recommended.



For more information on planning and installing EtherNet/IP networks, please refer to the "Media Planning and Installation Manual. EtherNet/IP" of ODVA Organization

*PROFINET*

Standard IEC 61156-6 specifies CAT 5 as the minimum category for a cable used for PROFINET. CAT 5e and CAT 6 are recommended.



For more information on planning and installing PROFINET networks, see: "PROFINET Cabling and Interconnection Technology", Guideline for PROFINET

*FOUNDATION Fieldbus*

Twisted, shielded two-wire cable.



For further information on planning and installing FOUNDATION Fieldbus networks see:

- Operating Instructions for "FOUNDATION Fieldbus Overview" (BA00013S)
- FOUNDATION Fieldbus Guideline
- IEC 61158-2 (MBP)

*Modbus RS485*

The EIA/TIA-485 standard specifies two types of cable (A and B) for the bus line which can be used for every transmission rate. Cable type A is recommended.

<b>Cable type</b>	A
<b>Characteristic impedance</b>	135 to 165 $\Omega$ at a measuring frequency of 3 to 20 MHz
<b>Cable capacitance</b>	< 30 pF/m
<b>Wire cross-section</b>	> 0.34 mm <sup>2</sup> (22 AWG)
<b>Cable type</b>	Twisted pairs
<b>Loop resistance</b>	$\leq 110 \Omega/\text{km}$
<b>Signal damping</b>	Max. 9 dB over the entire length of the cable cross-section
<b>Shield</b>	Copper braided shielding or braided shielding with foil shield. When grounding the cable shield, observe the grounding concept of the plant.

*Current output 0/4 to 20 mA*

Standard installation cable is sufficient.

*Pulse/frequency/switch output*

Standard installation cable is sufficient.

*Double pulse output*

Standard installation cable is sufficient.

*Relay output*

Standard installation cable is sufficient.

*Current input 0/4 to 20 mA*

Standard installation cable is sufficient.

*Status input*

Standard installation cable is sufficient.

**Connecting cable for transmitter - remote display and operating module DKX001***Standard cable*

A standard cable can be used as the connecting cable.

<b>Standard cable</b>	4 cores (2 pairs); pair-stranded with common shield
<b>Shielding</b>	Tin-plated copper-braid, optical cover $\geq 85 \%$
<b>Capacitance: core/shield</b>	Maximum 1 000 nF for Zone 1; Class I, Division 1

<b>L/R</b>	Maximum 24 $\mu\text{H}/\Omega$ for Zone 1; Class I, Division 1
<b>Cable length</b>	Maximum 300 m (1000 ft), see the following table

<b>Cross-section</b>	<b>Cable length for use in:</b> <ul style="list-style-type: none"> <li>■ Non-hazardous area</li> <li>■ Hazardous area: Zone 2; Class I, Division 2</li> <li>■ Hazardous area: Zone 1; Class I, Division 1</li> </ul>
0.34 mm <sup>2</sup> (22 AWG)	80 m (270 ft)
0.50 mm <sup>2</sup> (20 AWG)	120 m (400 ft)
0.75 mm <sup>2</sup> (18 AWG)	180 m (600 ft)
1.00 mm <sup>2</sup> (17 AWG)	240 m (800 ft)
1.50 mm <sup>2</sup> (15 AWG)	300 m (1000 ft)

#### Optionally available connecting cable

<b>Standard cable</b>	2 × 2 × 0.34 mm <sup>2</sup> (22 AWG) PVC cable <sup>1)</sup> with common shield (2 pairs, pair-stranded)
<b>Flame resistance</b>	According to DIN EN 60332-1-2
<b>Oil-resistance</b>	According to DIN EN 60811-2-1
<b>Shielding</b>	Tin-plated copper-braid, optical cover ≥ 85 %
<b>Capacitance: core/shield</b>	≤200 pF/m
<b>L/R</b>	≤24 $\mu\text{H}/\Omega$
<b>Available cable length</b>	10 m (35 ft)
<b>Operating temperature</b>	When mounted in a fixed position: -50 to +105 °C (-58 to +221 °F); when cable can move freely: -25 to +105 °C (-13 to +221 °F)

1) UV radiation can impair the cable outer sheath. Protect the cable from direct sunshine where possible.

## Performance characteristics

### Reference operating conditions

- Error limits following DIN EN 29104, in future ISO 20456
- Water, typically +15 to +45 °C (+59 to +113 °F); 0.5 to 7 bar (73 to 101 psi)
- Data as indicated in the calibration protocol
- Accuracy based on accredited calibration rigs according to ISO 17025

### Maximum measured error

#### Error limits under reference operating conditions


o.r. = of reading

#### Volume flow

- ±0.5 % o.r. ± 1 mm/s (0.04 in/s)
- Optional: ±0.2 % o.r. ± 2 mm/s (0.08 in/s)



Fluctuations in the supply voltage do not have any effect within the specified range.



A0028974

19 Maximum measured error in % o.r.

**Temperature**

$\pm 3\text{ }^{\circ}\text{C}$  ( $\pm 5.4\text{ }^{\circ}\text{F}$ )

**Electrical conductivity**

Max. measured error not specified.

**Accuracy of outputs**

The outputs have the following base accuracy specifications.

*Current output*

Accuracy	$\pm 5\text{ }\mu\text{A}$
----------	----------------------------

*Pulse/frequency output*

o.r. = of reading

Accuracy	Max. $\pm 50\text{ ppm o.r.}$ (over the entire ambient temperature range)
----------	---

**Repeatability**

o.r. = of reading

**Volume flow**

Max.  $\pm 0.1\text{ }\%$  o.r.  $\pm 0.5\text{ mm/s}$  ( $0.02\text{ in/s}$ )

**Temperature**

$\pm 0.5\text{ }^{\circ}\text{C}$  ( $\pm 0.9\text{ }^{\circ}\text{F}$ )

**Electrical conductivity**

- Max.  $\pm 5\text{ }\%$  o.r.
- Max.  $\pm 1\text{ }\%$  o.r. for DN 15 to 150 in conjunction with stainless steel process connections, 1.4404 (F316L)

**Temperature measurement response time**

$T_{90} < 15\text{ s}$

**Influence of ambient temperature**

**Current output**

Temperature coefficient	Max. $1\text{ }\mu\text{A}/^{\circ}\text{C}$
-------------------------	--


**Pulse/frequency output**

Temperature coefficient	No additional effect. Included in accuracy.
-------------------------	---

## Installation

No special measures such as supports etc. are necessary. External forces are absorbed by the construction of the device.

### Mounting location




A0029343

Preferably install the sensor in an ascending pipe, and ensure a sufficient distance to the next pipe elbow:  $h \geq 2 \times DN$

### Installation in down pipes

Install a siphon with a vent valve downstream of the sensor in down pipes whose length  $h \geq 5 \text{ m}$  (16.4 ft). This precaution is to avoid low pressure and the consequent risk of damage to the measuring tube. This measure also prevents the system losing prime.




A0028981

#### 20 Installation in a down pipe

- 1 Vent valve
- 2 Pipe siphon
- $h$  Length of down pipe

### Installation in partially filled pipes





A partially filled pipe with a gradient necessitates a drain-type configuration.



A0029257

### Orientation


The direction of the arrow on the sensor nameplate helps you to install the sensor according to the flow direction (direction of medium flow through the piping).

Orientation			Recommendation
A	Vertical orientation	 A0015591	✓✓
B	Horizontal orientation, transmitter at top	 A0015589	✓✓ <sup>1)</sup>
C	Horizontal orientation, transmitter at bottom	 A0015590	✓✓ <sup>2) 3)</sup>
D	Horizontal orientation, transmitter at side	 A0015592	✗

- 1) Applications with low process temperatures may decrease the ambient temperature. To maintain the minimum ambient temperature for the transmitter, this orientation is recommended.
- 2) Applications with high process temperatures may increase the ambient temperature. To maintain the maximum ambient temperature for the transmitter, this orientation is recommended.
- 3) To prevent the electronics module from overheating in the case of a sharp rise in temperature (e.g. CIP- or SIP processes), install the device with the transmitter component pointing downwards.

Horizontal

- Ideally, the measuring electrode plane should be horizontal. This prevents brief insulation of the two measuring electrodes by entrained air bubbles.
- Empty pipe detection only works if the transmitter housing is pointing upwards as otherwise there is no guarantee that the empty pipe detection function will actually respond to a partially filled or empty measuring tube.



- 1 EPD electrode for empty pipe detection (available from DN > 15 mm (½ in))
- 2 Measuring electrodes for signal detection


 Measuring devices with a nominal diameter < DN 15 mm (½ in) do not have an EPD electrode. In this case, empty pipe detection is performed via the measuring electrodes.

Inlet and outlet runs

If possible, install the sensor upstream from fittings such as valves, T-pieces or elbows.


Observe the following inlet and outlet runs to comply with accuracy specifications:





A0028997

- 21 Order code for "Design", option A "Insertion length short, ISO/DVGW until DN400, DN450-2000 1:1" and order code for "Design", option B "Insertion length long, ISO/DVGW until DN400, DN450-2000 1:1.3"



A0032859


- 22 Order code for "Design", option C "Insertion length short ISO/DVGW until DN300, w/o inlet and outlet runs, constricted meas.tube"

## Adapters

Suitable adapters to DIN EN 545 (double-flange reducers) can be used to install the sensor in larger-diameter pipes. The resultant increase in the rate of flow improves measuring accuracy with very slow-moving fluids.

The nomogram shown here can be used to calculate the pressure loss caused by reducers and expanders:

- Calculate the ratio of the diameters  $d/D$ .
- From the nomogram read off the pressure loss as a function of flow velocity (downstream from the reduction) and the  $d/D$  ratio.
- The nomogram only applies to liquids with a viscosity similar to that of water.
- If the medium has a high viscosity, a larger measuring tube diameter can be considered in order to reduce pressure loss.



A0029002

## Environment

Ambient temperature range	Transmitter	Standard: -40 to +60 °C (-40 to +140 °F)
	Local display	-20 to +60 °C (-4 to +140 °F), the readability of the display may be impaired at temperatures outside the temperature range.
	Sensor	-20 to +60 °C (-4 to +140 °F)
	Liner	Do not exceed or fall below the permitted temperature range of the liner .

If operating outdoors:

- Install the measuring device in a shady location.
- Avoid direct sunlight, particularly in warm climatic regions.
- Avoid direct exposure to weather conditions.



You can order a weather protection cover from Endress+Hauser : → 106

Storage temperature	-50 to +80 °C (-58 to +176 °F) <ul style="list-style-type: none"> <li>■ Protect the measuring device against direct sunlight during storage in order to avoid unacceptably high surface temperatures.</li> <li>■ Select a storage location where moisture cannot collect in the measuring device as fungus or bacteria infestation can damage the liner.</li> <li>■ If protection caps or protective covers are mounted these should never be removed before installing the measuring device.</li> </ul>
---------------------	--

Degree of protection	<b>Measuring device</b> <ul style="list-style-type: none"> <li>■ As standard: IP66/67, type 4X enclosure</li> <li>■ When housing is open: IP20, type 1 enclosure</li> <li>■ Display module: IP20, type 1 enclosure</li> <li>■ With the order code for "Sensor options", option <b>CM</b>: IP69 can also be ordered</li> </ul> <b>External WLAN antenna</b> IP67
----------------------	--

Vibration resistance	<ul style="list-style-type: none"> <li>■ Vibration, sinusoidal according to IEC 60068-2-6 <ul style="list-style-type: none"> <li>- 2 to 8.4 Hz, 3.5 mm peak</li> <li>- 8.4 to 2 000 Hz, 1 g peak</li> </ul> </li> <li>■ Vibration broad-band random, according to IEC 60068-2-64 <ul style="list-style-type: none"> <li>- 10 to 200 Hz, 0.003 g<sup>2</sup>/Hz</li> <li>- 200 to 2 000 Hz, 0.001 g<sup>2</sup>/Hz</li> <li>- Total: 1.54 g rms</li> </ul> </li> </ul>
----------------------	---

Shock resistance	Shock, half-sine according to IEC 60068-2-27 6 ms 50 g
------------------	---

Impact resistance	Rough handling shocks according to IEC 60068-2-31
-------------------	---

Mechanical load	<ul style="list-style-type: none"> <li>■ Protect the transmitter housing against mechanical effects, such as shock or impact.</li> <li>■ Never use the transmitter housing as a ladder or climbing aid.</li> </ul>
-----------------	--

Interior cleaning	<ul style="list-style-type: none"> <li>■ Cleaning in place (CIP)</li> <li>■ Sterilization in place (SIP)</li> </ul>
-------------------	---


Electromagnetic compatibility (EMC)	As per IEC/EN 61326 and NAMUR Recommendation 21 (NE 21)
-------------------------------------	---



Details are provided in the Declaration of Conformity.

## Process

**Medium temperature range**     -20 to +150 °C (-4 to +302 °F)




$T_A$     Ambient temperature range  
 $T_F$     Fluid temperature

**Conductivity**      $\geq 5 \mu\text{S/cm}$  for liquids in general. Stronger filter damping is required for very low conductivity values.

**Pressure-temperature ratings**     The following graphics contain material load diagrams (reference curves) for different process connections in relation to the medium temperature.


### Process connections with O-ring seal, DN 2 to 25 (1/12 to 1")

Process connection: weld-in nipple according to DIN EN ISO 1127, ODT/SMS, ISO 2037; coupling according to ISO 228 / DIN 2999, NPT




23    Process connection material: stainless steel, 1.4404 (F316L)


Process connection: flange according to EN 1092-1 (DIN 2501), adhesive sleeve



24 Process connection material: stainless steel, 1.4404 (F316L)




25 Process connection material: PVDF




26 Process connection material: PVC-U

Process connection: flange according to ASME B16.5




27 Process connection material: stainless steel, 1.4404 (F316L)




28 Process connection material: PVDF

Process connection: flange according to JIS B2220



29 Process connection material: stainless steel, 1.4404 (F316L)




A0028939-EN

30 Process connection material: PVDF

**Process connections with aseptic gasket seal, DN 2 to 25 (1/12 to 1")**

Process connection: weld-in nipple according to EN 10357 (DIN 11850), ASME BPE, ISO 2037; clamp according to ISO 2852, DIN 32676; coupling according to SC DIN 11851, DIN 11864-1, SMS 1145; flange according to DIN 11864-2




A0028940-EN

31 Process connection material: stainless steel, 1.4404 (F316L)

**Process connections with aseptic gasket seal, DN 40 to 150 (1 ½ to 6")**


Process connection: coupling according to SMS 1145



A0028940-EN


32 Process connection material: stainless steel, 1.4404 (F316L)

Process connection: weld-in nipple according to EN 10357 (DIN 11850); coupling according to SC DIN 11851




33 Process connection material: stainless steel, 1.4404 (F316L)

Process connection: weld-in nipple according to ASME BPE




Process connection: weld-in nipple according to ISO 2037




34 Process connection material: stainless steel, 1.4404 (F316L)

Process connection: clamp according to ISO 2852, DIN 32676



35 Process connection material: stainless steel, 1.4404 (F316L)


Process connection: coupling according to DIN 11864-1, ISO 2853



36 Process connection material: stainless steel, 1.4404 (F316L)



Process connection: flange according to DIN 11864-2



37 Process connection material: stainless steel, 1.4404 (F316L)

A0028945-EN

Pressure tightness

Liner: PFA

Nominal diameter		Limit values for absolute pressure in [mbar] ([psi]) for medium temperatures:				
[mm]	[in]	+25 °C (+77 °F)	+80 °C (+176 °F)	+100 °C (+212 °F)	+130 °C (+266 °F)	+150 °C (+302 °F)
2 to 150	1/12 to 6	0 (0)	0 (0)	0 (0)	0 (0)	0 (0)

Flow limit

The diameter of the pipe and the flow rate determine the nominal diameter of the sensor. The optimum velocity of flow is between 2 to 3 m/s (6.56 to 9.84 ft/s). Also match the velocity of flow (v) to the physical properties of the fluid:


- $v < 2$  m/s (6.56 ft/s): for low conductivity values
- $v > 2$  m/s (6.56 ft/s): for fluids producing buildup (e.g. milk with a high fat content)

**i** A necessary increase in the flow velocity can be achieved by reducing the sensor nominal diameter.


**i** For an overview of the full scale values for the measuring range, see the "Measuring range" section → 9

Pressure loss

- No pressure loss occurs as of nominal diameter DN 8 (5/16") if the sensor is installed in a pipe with the same nominal diameter.
- Pressure losses for configurations incorporating adapters according to DIN EN 545 → 45




38 Pressure loss DN 50 to 80 (2 to 3") in the case of order code for "Design", option C "Insertion length short ISO/DVGW to DN300, without inlet/outlet runs, constricted meas.tube"



39 Pressure loss DN 100 to 300 (4 to 12") in the case of order code for "Design", option C "Insertion length short ISO/DVGW to DN300, without inlet/outlet runs, constricted meas.tube"

System pressure




Never install the sensor on the pump suction side in order to avoid the risk of low pressure, and thus damage to the liner.

**i** Furthermore, install pulse dampers if reciprocating, diaphragm or peristaltic pumps are used.

- i** ■ Information on the liner's resistance to partial vacuum → 53
- Information on the shock resistance of the measuring system → 46
- Information on the vibration resistance of the measuring system → 46

Vibrations



40 Measures to avoid device vibrations ( $L > 10\text{ m}$  (33 ft))


In the event of very strong vibrations, the pipe and sensor must be supported and fixed.

- i** ■ Information on the shock resistance of the measuring system → 46
- Information on the vibration resistance of the measuring system → 46

Mechanical construction

Dimensions in SI units

Compact version



Order code for "Housing", option A "Aluminum, coated"

DN	A <sup>1)</sup>	B <sup>1)</sup>	C	D	E	F	G <sup>2)</sup>	H	I <sup>2)</sup>	K	L <sup>3)</sup>	M
[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]
2	169	68	101	55	240	295	200	59	141	2.25	86	43
4	169	68	101	55	240	295	200	59	141	4.5	86	43
8	169	68	101	55	240	295	200	59	141	9	86	43
15	169	68	101	55	240	295	200	59	141	16	86	43
25	169	68	101	55	240	295	200	59	141	26	86	56

DN	A <sup>1)</sup>	B <sup>1)</sup>	C	D	E	F	G <sup>2)</sup>	H	I <sup>2)</sup>	K	L <sup>3)</sup>	M
[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]
40	169	68	101	54	239	293	200	59	141	34.8	140	107
50	169	68	101	60	246	306	200	59	141	47.5	140	120
65	169	68	101	68	254	322	200	59	141	60.2	140	135
80	169	68	101	74	260	334	200	59	141	72.9	140	148
100	169	68	101	87	273	360	200	59	141	97.4	140	174
125	169	68	101	103	289	392	200	59	141	120.0	200	206
150	169	68	101	117	303	420	200	59	141	146.9	200	234

- 1) Depending on the cable gland used: values up to + 30 mm  
2) For version without local display: values – 30 mm  
3) Total length (L) depends on the process connections.

Order code for "Housing", option A "Aluminum, coated"; Ex d

DN	A <sup>1)</sup>	B <sup>1)</sup>	C	D	E	F	G <sup>2)</sup>	H	I <sup>2)</sup>	K	L <sup>3)</sup>	M
[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]
2	188	85	103	55	269	324	206	58	148	2.25	86	43
4	188	85	103	55	269	324	206	58	148	4.5	86	43
8	188	85	103	55	269	324	206	58	148	9	86	43
15	188	85	103	55	269	324	206	58	148	16	86	43
25	188	85	103	55	269	324	206	58	148	26	86	56
40	188	85	103	54	270	324	206	58	148	34.8	140	107
50	188	85	103	60	276	336	206	58	148	47.5	140	120
65	188	85	103	67	284	351	206	58	148	60.2	140	135
80	188	85	103	74	290	364	206	58	148	72.9	140	148
100	188	85	103	87	303	390	206	58	148	97.4	140	174
125	188	85	103	103	319	422	206	58	148	120.0	200	206
150	188	85	103	117	333	450	206	58	148	146.9	200	234

- 1) Depending on the cable gland used: values up to + 30 mm  
2) For version without local display: values – 30 mm  
3) Total length (L) depends on the process connections.


Order code for "Housing", option B "Stainless, hygienic"

DN	A <sup>1)</sup>	B <sup>1)</sup>	C	D	E	F	G <sup>2)</sup>	H	I <sup>2)</sup>	K	L <sup>3)</sup>	M
[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]
2	183	73	110	55	254	309	207	65	142	2.25	86	43
4	183	73	110	55	254	309	207	65	142	4.5	86	43
8	183	73	110	55	254	309	207	65	142	9	86	43
15	183	73	110	55	254	309	207	65	142	16	86	43
25	183	73	110	55	254	309	207	65	142	26	86	56
40	183	73	110	54	255	309	207	65	142	34.8	140	107
50	183	73	110	60	261	321	207	65	142	47.5	140	120
65	183	73	110	67	269	336	207	65	142	60.2	140	135
80	183	73	110	74	275	349	207	65	142	72.9	140	148

DN	A <sup>1)</sup>	B <sup>1)</sup>	C	D	E	F	G <sup>2)</sup>	H	I <sup>2)</sup>	K	L <sup>3)</sup>	M
[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]
100	183	73	110	87	288	375	207	65	142	97.4	140	174
125	183	73	110	103	304	407	207	65	142	120.0	200	206
150	183	73	110	117	318	435	207	65	142	146.9	200	234


- 1) Depending on the cable gland used: values up to + 30 mm  
2) For version without local display: values – 30 mm  
3) Total length (L) depends on the process connections.

Sensor flange connection



41 Front view without process connections

DN	A	B	C	D	E	F	G	H	K	L	M
[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]
2	62	41.6	34	9	24	42	43	8.5	6	4	M6
4	62	41.6	34	9	24	42	43	8.5	6	4	M6
8	62	41.6	34	9	24	42	43	8.5	6	4	M6
15	62	41.6	34	16	24	42	43	8.5	6	4	M6
25	72	50.2	44	26	29	55	56	8.5	6	4	M6




A0005528

42 Front view without process connections

DN	A	B	C	D	E	F	G	H	K	L
									$90^\circ \pm 0.5^\circ$	$60^\circ \pm 0.5^\circ$
	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	Tapped holes	
40	99.7	85.8	71.0	48.3	34.8	M8	12	17	4	–
50	112.7	98.8	83.5	60.3	47.5	M8	12	17	4	–
65	127.7	114.8	100.0	76.1	60.2	M8	12	17	–	6
80	140.7	133.5	114.0	88.9	72.9	M8	12	17	–	6
100	166.7	159.5	141.0	114.3	97.4	M8	12	17	–	6
125	198.7	191.5	171.0	139.7	120.0	M10	15	20	–	6
150	226.7	219.5	200.0	168.3	146.9	M10	15	20	–	6

### Flange connections

Flanges with aseptic gasket seal



A0015627

43 Detail X: Asymmetrical process connection; the part shown in gray is provided by the supplier.

**Flange DIN 11864-2, aseptic female, Form A**  
**1.4404 (316L)**
*Order code for "Process connection", option DES*

DN [mm]	Suitable for pipe EN 10357 (DIN 11850) [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
2 to 8	13 × 1.5 (DN 10)	54	37	4 × Ø9	10	10	183
15	19 × 1.5 (DN 15)	59	42	4 × Ø9	10	16	183
25	29 × 1.5 (DN 25)	70	53	4 × Ø9	10	26	183

 Surface roughness:  $R_a \leq 0.8 \mu\text{m}$ , optional  $\leq 0.38 \mu\text{m}$ 


Please note the internal diameters of the measuring tube and process connection (E) when cleaning with pigs.

**Flange DIN 11864-2, aseptic flange with notch, Form A**  
**1.4404 (316L)**
*Order code for "Process connection", option DES*

DN [mm]	Suitable for pipe EN 10357 (DIN 11850) [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
40	41 × 1.5	82	65	4 × Ø9	10	38	246
50	53 × 1.5	94	77	4 × Ø9	10	50	246
65	70 × 2	113	95	8 × Ø9	10	66	246
80	85 × 2	133	112	8 × Ø11	10	81	270
100	104 × 2	159	137	8 × Ø11	10	100	278
125	129 × 2	183	161	8 × Ø11	10	125	362
150	154 × 2	213	188	8 × Ø14	10	150	362

 Surface roughness:  $R_a \leq 0.8 \mu\text{m}$ , optional  $\leq 0.38 \mu\text{m}$ 

Please note the internal diameters of the measuring tube and process connection (E) when cleaning with pigs.

*Flanges with O-ring seal*


A0015621

**Flange according to EN 1092-1 (DIN 2501), Form B: PN 40**  
**1.4404 (316L)**
*Order code for "Process connection", option D5S*

DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
2 to 8 <sup>1)</sup>	95	65	4 × Ø14	16	17.3	198.4
15	95	65	4 × Ø14	16	17.3	198.4

**Flange according to EN 1092-1 (DIN 2501), Form B: PN 40  
1.4404 (316L)**
*Order code for "Process connection", option D5S*

DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
25	115	85	4 × Ø14	18	28.5	198.4

 Surface roughness:  $R_a \leq 1.6 \mu\text{m}$ 

- 1) DN 2 to 8 with DN 15 flanges as standard

**Flange according to ASME B16.5: Class 150  
1.4404 (316L)**
*Order code for "Process connection", option A1S*

DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
2 to 8 <sup>1)</sup>	90	60.3	4 × Ø15.7	11.2	15.7	218
15	90	60.3	4 × Ø15.7	11.2	15.7	218
25	110	79.4	4 × Ø15.7	14.2	26.7	230

 Surface roughness:  $R_a \leq 1.6 \mu\text{m}$ 


- 1) DN 2 to 8 with DN 15 flanges as standard

**Flange according to JIS B2220: 20K  
1.4404 (316L)**
*Order code for "Process connection", option N4S*

DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
2 to 8 <sup>1)</sup>	95	70	4 × Ø15	14	15	220
15	95	70	4 × Ø15	14	15	220
25	125	90	4 × Ø19	16	25	220

 Surface roughness:  $R_a \leq 1.6 \mu\text{m}$ 

- 1) DN 2 to 8 with DN 15 flanges as standard



A0022221



**Lap joint flange according to EN 1092-1 (DIN 2501): PN 16**  
**PVDF**
*Order code for "Process connection", option D3P*

DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	F [mm]	L [mm]
2 to 8 <sup>1)</sup>	95	65	4 x Ø14	14.5	45	17.3	200
15	95	65	4 x Ø14	14.5	45	17.3	200
25	115	85	4 x Ø14	16.5	68	28.5	200

 Surface roughness:  $R_a \leq 1.6 \mu\text{m}$ 

The required grounding rings can be ordered as accessories (order code: DK5HR-\*\*\*\*).

- 1) DN 2 to 8 with DN 15 flanges as standard

**Lap joint flange with grounding electrode according to EN 1092-1 (DIN 2501): PN 16**  
**PVDF**
*Order code for "Process connection", option D4P*

DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	F [mm]	L [mm]
2 to 8 <sup>1)</sup>	95	65	4 x Ø14	14.5	45	17.3	200
15	95	65	4 x Ø14	14.5	45	17.3	200
25	115	85	4 x Ø14	16.5	68	28.5	200

 Surface roughness:  $R_a \leq 1.6 \mu\text{m}$ 

Grounding rings are not necessary.

- 1) DN 2 to 8 with DN 15 flanges as standard

**Lap joint flange according to ASME B16.5: Class 150**  
**PVDF**
*Order code for "Process connection", option A1P*

DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	F [mm]	L [mm]
2 to 8 <sup>1)</sup>	90	60.3	4 × Ø 15.7	15	35.1	15.7	200
15	90	60.3	4 × Ø 15.7	15	35.1	15.7	200
25	110	79.4	4 × Ø 15.7	16	50.8	26.7	200

 Surface roughness:  $R_a \leq 1.6 \mu\text{m}$ 

The required grounding rings can be ordered as accessories (order code: DK5HR-\*\*\*\*).

- 1) DN 2 to 8 with DN 15 flanges as standard

**Lap joint flange with grounding electrode according to ASME B16.5: Class 150**  
**PVDF**
*Order code for "Process connection", option A4P*

DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	F [mm]	L [mm]
2 to 8 <sup>1)</sup>	90	60.3	4 × Ø 15.7	15	35.1	15.7	200
15	90	60.3	4 × Ø 15.7	15	35.1	15.7	200
25	110	79.4	4 × Ø 15.7	16	50.8	26.7	200

 Surface roughness:  $R_a \leq 1.6 \mu\text{m}$ 

Grounding rings are not necessary.

- 1) DN 2 to 8 with DN 15 flanges as standard

**Lap joint flange according to JIS B2220: 10K  
PVDF**
*Order code for "Process connection", option N3P*

DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	F [mm]	L [mm]
2 to 8 <sup>1)</sup>	95	70	4 × Ø 15.7	15	35.1	15	200
15	95	70	4 × Ø 15.7	15	35.1	15	200
25	125	90	4 × Ø 15.7	16	50.8	19	200

 Surface roughness:  $R_a \leq 1.6 \mu\text{m}$ 

The required grounding rings can be ordered as accessories (order code: DK5HR-\*\*\*\*).

- 1) DN 2 to 8 with DN 15 flanges as standard


**Lap joint flange with grounding electrode according to JIS B2220: 10K  
PVDF**
*Order code for "Process connection", option N4P*

DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	F [mm]	L [mm]
2 to 8 <sup>1)</sup>	95	70	4 × Ø 15.7	15	35.1	15	200
15	95	70	4 × Ø 15.7	15	35.1	15	200
25	125	90	4 × Ø 15.7	16	50.8	19	200

 Surface roughness:  $R_a \leq 1.6 \mu\text{m}$ 

Grounding rings are not necessary.

- 1) DN 2 to 8 with DN 15 flanges as standard

**Welding nipple**
*Welding nipple with aseptic gasket seal*


A0027510

**Welding nipple according to EN 10357 (DIN 11850)  
1.4404 (316L)**
*Order code for "Process connection", option DAS*

DN [mm]	Suitable for pipe EN 10357 (DIN 11850) [mm]	A [mm]	B [mm]	L [mm]
2 to 8	13 × 1.5	13	10	132.6
15	19 × 1.5	19	16	132.6
25	29 × 1.5	29	26	132.6
40	41 × 1.5	41	38	220
50	53 × 1.5	53	50	220
65	70 × 2	70	66	220
80	85 × 2	85	81	220

**Welding nipple according to EN 10357 (DIN 11850)**  
**1.4404 (316L)**
*Order code for "Process connection", option DAS*

DN [mm]	Suitable for pipe EN 10357 (DIN 11850) [mm]	A [mm]	B [mm]	L [mm]
100	104 × 2	104	100	220
125	129 × 2	129	125	300
150	154 × 2	154	150	300

 Surface roughness:  $R_a \leq 0.8 \mu\text{m}$ , optional  $\leq 0.38 \mu\text{m}$ 

Please note the internal diameters of the measuring tube and process connection (B) when cleaning with pigs.

**Welding nipple according to ISO 2037**  
**1.4404 (316L)**
*Order code for "Process connection", option IAS*

DN [mm]	Suitable for pipe ISO 2037 [mm]	A [mm]	B [mm]	L [mm]
2 to 8	12.7 × 1.65	12	10	118.2
15	19.05 × 1.65	18	16	118.2
25	25.4 × 1.60	25	22.6	118.2
40	38 × 1.2	38	35.6	220
50	51 × 1.2	51	48.6	220
65	63.5 × 1.6	63.5	60.3	220
80	76.1 × 1.6	76.1	72.9	220
100	101.6 × 2	101.6	97.6	220
125	139.7 × 2	139.7	135.7	380
150	168.3 × 2.6	168.3	163.1	380

 Surface roughness:  $R_a \leq 0.8 \mu\text{m}$ , optional  $\leq 0.38 \mu\text{m}$ 

Please note the internal diameters of the measuring tube and process connection (B) when cleaning with pigs.


**Welding nipple according to ASME BPE**  
**1.4404 (316L)**
*Order code for "Process connection", option AAS*

DN [mm]	Suitable for pipe ASME BPE [mm]	A [mm]	B [mm]	L [mm]
2 to 8	12.7 × 1.65	12.7	9	118.2
15	19.1 × 1.65	19.1	16	118.2
25	25.4 × 1.65	25.4	22.6	118.2
40	38.1 × 1.65	38.1	34.8	220
50	50.8 × 1.65	50.8	47.5	220
65	63.5 × 1.65	63.5	60.2	220
80	76.2 × 1.65	76.2	72.9	220
100	101.6 × 1.65	101.6	97.4	220
150	152.4 × 2.77	149.9	149.9	300

 Surface roughness:  $R_a \leq 0.8 \mu\text{m}$ , optional  $\leq 0.38 \mu\text{m}$ 

Please note the internal diameters of the measuring tube and process connection (B) when cleaning with pigs.

## Welding nipple with O-ring seal



A0027510

## Welding nipple according to ODT/SMS

1.4404 (316L)

Order code for "Process connection", option A2S

DN [mm]	Suitable for pipe ODT/SMS [mm]	A [mm]	B [mm]	L [mm]
2 to 8	13.5 × 2.30	13.5	9	126.6
15	21.3 × 2.65	21.3	16	126.6
25	33.7 × 3.25	33.7	27.2	126.6

Surface roughness:  $R_a \leq 1.6 \mu\text{m}$ 

## Welding nipple according to DIN EN ISO 1127

1.4404 (316L)

Order code for "Process connection", option D1S

DN [mm]	Suitable for pipe DIN EN ISO 1127 [mm]	A [mm]	B [mm]	L [mm]
2 to 8	13.5 × 1.6	13.5	10.3	126.6
15	21.3 × 1.6	21.3	18.1	126.6
25	33.7 × 2.0	33.7	29.7	126.6

Surface roughness:  $R_a \leq 1.6 \mu\text{m}$ 

## Welding nipple according to ISO 2037

1.4404 (316L)


Order code for "Process connection", option I1S

DN [mm]	Suitable for pipe ISO 2037 [mm]	A [mm]	B [mm]	L [mm]
2 to 8	13.5 × 2.3	13.5	9	126.6
15	21.3 × 2.65	21.3	16	126.6
25	33.7 × 3.25	33.7	27.2	126.6

Surface roughness:  $R_a \leq 1.6 \mu\text{m}$

## Clamp connections

### Clamp connections with aseptic gasket seal



A0015625

#### Clamp according to DIN 32676

**1.4404 (316L)**
*Order code for "Process connection", option DBS*

DN [mm]	Suitable for pipe EN 10357 (DIN 11850) [mm]	A [mm]	B [mm]	L [mm]
2 to 8	14 × 2 (DN 10)	34	10	168
15	20 × 2 (DN 15)	34	16	168
25	30 × 2 (DN 25)	50.5	26	175
40	41 × 1.5	50.5	38	220
50	53 × 1.5	64	50	220
65	70 × 2	91	66	220
80	85 × 2	106	81	220
100	104 × 2	119	100	220
125	129 × 2	155	125	300
150	154 × 2	183	150	300

 Surface roughness:  $R_a \leq 0.8 \mu\text{m}$ , optional  $\leq 0.38 \mu\text{m}$ 

Please note the internal diameters of the measuring tube and process connection (B) when cleaning with pigs.

#### Tri-Clamp

**1.4404 (316L)**
*Order code for "Process connection", option FAS*

DN [mm]	Suitable for pipe as per ASME BPE [mm]	A [mm]	B [mm]	L [mm]
2 to 8	12.7 × 1.65	25	9.4	143
15	19.1 × 1.65	25	15.8	143
25	25.4 × 1.65	50.4	22.1	143
40	38.1 × 1.65	50.4	34.8	220
50	50.8 × 1.65	63.9	47.5	220
65	63.5 × 1.65	77.4	60.2	220
80	76.2 × 1.65	90.9	72.9	220
100	101.6 × 2.11	118.9	97.4	220
150	152.4 × 2.77	166.9	146.9	300

 Surface roughness:  $R_a \leq 0.8 \mu\text{m}$ , optional  $\leq 0.38 \mu\text{m}$ 


Please note the internal diameters of the measuring tube and process connection (B) when cleaning with pigs.

**Clamp according to ISO 2852, Fig. 2**  
**1.4404 (316L)**
*Order code for "Process connection", option IBS*

DN [mm]	Suitable for pipe ISO 2037 [mm]	A [mm]	B [mm]	L [mm]
25	24.5 × 1.65	50.5	22.6	174.6
40	38 × 1.6	50.5	35.6	220
50	51 × 1.6	64	48.6	220
65	63.5 × 1.6	77.5	60.3	220
80	76.1 × 1.6	91	72.9	220
100	101.6 × 2	119	97.6	220
125	139.7 × 2	155	135.7	300
150	168.3 × 2.6	183	163.1	300

 Surface roughness:  $R_a \leq 0.8 \mu\text{m}$ , optional  $\leq 0.38 \mu\text{m}$ 

Please note the internal diameters of the measuring tube and process connection (B) when cleaning with pigs.

**Threaded glands**
*Thread with aseptic gasket seal*


A0027509

**Coupling SC DIN 11851, thread**  
**1.4404 (316L)**
*Order code for "Process connection", option DCS*

DN [mm]	Suitable for pipe EN 10357 (DIN 11850) [mm]	A [mm/in]	B [mm]	L [mm]
2 to 8	12 × 1 (DN 10)	Rd 28 × 1/8	10	174
15	18 × 1.5 (ODT 3/4")	Rd 34 × 1/8	16	174
25	28 × 1 or 28 × 1.5	Rd 52 × 1/6	26	190
40	41 × 1.5	Rd 65 × 1/6	38	260
50	53 × 1.5	Rd 78 × 1/6	50	260
65	70 × 2	Rd 95 × 1/6	66	270
80	85 × 2	Rd 110 × 1/4	81	280
100	104 × 2	Rd 130 × 1/4	100	290
125	129 × 2	Rd 160 × 1/4	125	380
150	154 × 2	Rd 160 × 1/4	150	390

 Surface roughness:  $R_a \leq 0.8 \mu\text{m}$ , optional  $\leq 0.38 \mu\text{m}$ 


Please note the internal diameters of the measuring tube and process connection (B) when cleaning with pigs.

Coupling DIN 11864-1, aseptic thread, Form A 1.4404 (316L) Order code for "Process connection", option DDS				
DN [mm]	Suitable for pipe EN 10357 (DIN 11850) [mm]	A [mm/in]	B [mm]	L [mm]
2 to 8	Pipe 13 × 1.5 (DN 10)	Rd 28 × 1/8	10	170
15	Pipe 19 × 1.5	Rd 34 × 1/8	16	170
25	Pipe 29 × 1.5	Rd 52 × 1/6	26	184
40	41 × 1.5	Rd 65 × 1/6	38	256
50	53 × 1.5	Rd 78 × 1/6	50	256
65	70 × 2	Rd 95 × 1/6	66	266
80	85 × 2	Rd 110 × 1/4	81	276
100	104 × 2	Rd 130 × 1/4	100	286
Surface roughness: R <sub>a</sub> ≤ 0.8 μm, optional ≤ 0.38 μm Please note the internal diameters of the measuring tube and process connection (B) when cleaning with pigs.				

Coupling ISO 2853, thread 1.4404 (316L) Order code for "Process connection", option ICS					
DN [mm]	Suitable for pipe ISO 2037 [mm]	DN Clamp ISO 2853 [mm]	A [mm/in]	B [mm]	L [mm]
40	38 × 1.6	38	Tr 50.5 × 3.175	35.6	256
50	51 × 1.6	51	Tr 64 × 3.175	48.6	256
65	63.5 × 1.6	63.5	Tr 77.5 × 3.175	60.3	266
80	76.1 × 1.6	76.1	Tr 91 × 3.175	72.9	276
100	101.6 × 2	101.6	Tr 118 × 3.175	97.6	286
Surface roughness: $R_a \leq 0.8 \mu\text{m}$ , optional $\leq 0.38 \mu\text{m}$ Please note the internal diameters of the measuring tube and process connection (B) when cleaning with pigs.					

Coupling SMS 1145, thread 1.4404 (316L) Order code for "Process connection", option SAS					
DN [mm]	Suitable for pipe ODT [mm]	DN SMS 1145 [mm]	A [mm/in]	B [mm]	L [mm]
25	1	25	Rd40 × 1/6	22.6	147.6
40	38.1 × 1.65	38	Rd 60 × 1/6"	34.8	256
50	50.8 × 1.65	51	Rd 70 × 1/6"	47.5	256
65	63.5 × 1.65	63.5	Rd 85 × 1/6"	60.2	266
80	76.2 × 1.65	76	Rd 98 × 1/6"	72.6	276
100	101.6 × 1.65	101.6	Rd 132 × 1/6"	97.4	286
Surface roughness: $R_a \leq 0.8 \mu\text{m}$ , optional $\leq 0.38 \mu\text{m}$ Please note the internal diameters of the measuring tube and process connection (B) when cleaning with pigs.					

Thread with O-ring seal




A0027509

External thread according to ISO 228/DIN 2999 1.4404 (316L) Order code for "Process connection", option I2S			
DN [mm]	A [mm/in]	B [mm]	L [mm]
2 to 8	R 10.1 × 3/8	10	166
15	R 13.2 × ½	16	166
25	R 16.5 × 1	25	170
Surface roughness: R <sub>a</sub> ≤ 1.6 µm			

Internal thread according to ISO 228/DIN 2999 1.4404 (316L) Order code for "Process connection", option I3S			
DN [mm]	A [mm/in]	B [mm]	L [mm]
2 to 8	Rp 13 × 3/8	9	176
15	Rp 14 × ½	16	176
25	Rp 17 × 1	27.2	188
Surface roughness: R <sub>a</sub> ≤ 1.6 µm			

Hose adapter

Hose adapter with O-ring seal




A0027511



<b>Hose adapter</b> <b>1.4404 (316L)</b> <i>Order code for "Process connection", options O1S, O2S, O3S</i>			
<b>DN</b> <b>[mm]</b>	<b>Suitable for internal diameter</b> <b>[mm]</b>	<b>A</b> <b>[mm]</b>	<b>L</b> <b>[mm]</b>
2 to 8	13	10	184
15	16	12.6	184
25	19	16	184
Surface roughness: $R_a \leq 1.6 \mu\text{m}$			

**Adhesive sleeves**

*Adhesive sleeves with O-ring seal*




A0027510

<b>Adhesive sleeve</b> <b>PVC</b> <i>Order code for "Process connection", options O1V, O2V</i>				
<b>DN</b> <b>[mm]</b>	<b>Suitable for pipe</b> <b>[mm] / [in]</b>	<b>A</b> <b>[mm]</b>	<b>B</b> <b>[mm]</b>	<b>L</b> <b>[mm]</b>
2 to 8	20 × 2 (DIN 8062)	27	20.2	163
15	½	27.3	21.5	163
25	20 × 2 (DIN 8062)	27	20.2	142
Surface roughness: $R_a \leq 1.6 \mu\text{m}$ The required grounding rings can be ordered as accessories (order code: DK5HR-****).				

Mounting kits

Wall mounting kit




A0005537

A [mm]	B [mm]	C [mm]	Ø D [mm]	E [mm]	F [mm]
137	110	120	7	125	88


Accessories

Protective cover



A0029553

Remote display and operating module DKX001




A0028921

44 Engineering unit mm (in)

External WLAN antenna

External WLAN antenna mounted on device




A0028923

45 Engineering unit mm (in)


External WLAN antenna mounted with cable

The external WLAN antenna can be mounted separately from the transmitter if the transmission/reception conditions at the transmitter mounting location are poor.




46 Engineering unit mm (in)

Spacer



Order code: DK5HB-****				
DN [mm]	di [mm]	D1 [mm]	D2 [mm]	L [mm]
80	72.9	140.7	141	30
100	97.4	166.7	162	30

Clamp connections with aseptic gasket seal available for order




**Tri-Clamp**  
**1.4404 (316L)**  
**Order code: DKH\*\*-HF\*\***

DN [mm]	Suitable for pipe in accordance with ASME BPE (reduction) [mm]	A [mm]	B [mm]	L [mm]
15	Pipe ODT 1	50.4	22.1	143

Surface roughness:  $R_a \leq 0.8 \mu\text{m}$ , optional  $\leq 0.38 \mu\text{m}$

Please note the internal diameters of the measuring tube and process connection (B) when cleaning with pigs.

*Threaded glands with O-ring seal available for order*



A0027509

**External thread**  
**1.4404 (316L)**  
**Order code: DKH\*\*-GD\*\***

DN [mm]	Suitable for NPT internal thread [in]	A [mm/in]	B [mm]	L [mm]
2 to 8	NPT 3/8	R 15.5 × 3/8	10	186
15	NPT 1/2	R 20 × 1/2	16	186
25	NPT 1	R 25 × 1	25	196


Surface roughness:  $R_a \leq 1.6 \mu\text{m}$

**Internal thread**  
**1.4404 (316L)**  
**Order code: DKH\*\*-GC\*\***

DN [mm]	Suitable for NPT external thread [in]	A [mm/in]	B [mm]	L [mm]
2 to 8	NPT 3/8	R 13 × 3/8	8.9	176
15	NPT 1/2	R 14 × 1/2	16	176
25	NPT 1	R 17 × 1	27.2	188

Surface roughness:  $R_a \leq 1.6 \mu\text{m}$

Grounding rings




A0017673

For lap joint flange made of PVDF and PVC adhesive sleeve  
1.4435 (316L), Alloy C22, tantalum  
Order code: DK5HR-\*\*\*\*

DN [mm]	di [mm]	B [mm]	C [mm]	D [mm]	E [mm]	F [mm]	G [mm]	H [mm]	J [mm]
2 to 8	9	22	17.6	33.9	0.5	3.5	1.9	3.4	4.5
15	16	29	24.6	33.9	0.5	3.5	1.9	3.4	4.5
25	26	39	34.6	43.9	0.5	3.5	1.9	3.4	4.5

Dimensions in US units

Compact version



A0033785

Order code for "Housing", option A "Aluminum, coated"

DN [in]	A <sup>1)</sup> [in]	B <sup>1)</sup> [in]	C [in]	D [in]	E [in]	F [in]	G <sup>2)</sup> [in]	H [in]	I <sup>2)</sup> [in]	K [in]	L <sup>3)</sup> [in]	M [in]
1/12	6.65	2.68	3.98	2.17	9.45	11.6	7.87	2.32	5.55	0.09	3.39	1.69
1/8	6.65	2.68	3.98	2.17	9.45	11.6	7.87	2.32	5.55	0.18	3.39	1.69
3/8	6.65	2.68	3.98	2.17	9.45	11.6	7.87	2.32	5.55	0.35	3.39	1.69
1/2	6.65	2.68	3.98	2.17	9.45	11.6	7.87	2.32	5.55	0.63	3.39	1.69
1	6.65	2.68	3.98	2.17	9.45	11.6	7.87	2.32	5.55	1.02	3.39	2.20

DN [in]	A <sup>1)</sup> [in]	B <sup>1)</sup> [in]	C [in]	D [in]	E [in]	F [in]	G <sup>2)</sup> [in]	H [in]	I <sup>2)</sup> [in]	K [in]	L <sup>3)</sup> [in]	M [in]
1 ½	6.65	2.68	3.98	2.13	9.41	11.5	7.87	2.32	5.55	1.37	5.51	4.21
2	6.65	2.68	3.98	2.36	9.69	12.1	7.87	2.32	5.55	1.87	5.51	4.72
3	6.65	2.68	3.98	2.91	10.2	13.2	7.87	2.32	5.55	2.87	5.51	5.83
4	6.65	2.68	3.98	3.43	10.8	14.2	7.87	2.32	5.55	3.83	5.51	6.85
6	6.65	2.68	3.98	4.61	11.9	16.5	7.87	2.32	5.55	5.78	7.87	9.21

- 1) Depending on the cable gland used: values up to + 1.18 in  
 2) For version without local display: values – 1.18 in  
 3) Total length (L) depends on the process connections.

*Order code for "Housing", option A "Aluminum, coated"; Ex d*

DN [in]	A <sup>1)</sup> [in]	B <sup>1)</sup> [in]	C [in]	D [in]	E [in]	F [in]	G <sup>2)</sup> [in]	H [in]	I <sup>2)</sup> [in]	K [in]	L <sup>3)</sup> [in]	M [in]
¼	7.40	3.35	4.06	2.17	10.6	12.8	8.11	2.28	5.83	0.09	3.39	1.69
⅜	7.40	3.35	4.06	2.17	10.6	12.8	8.11	2.28	5.83	0.18	3.39	1.69
¾	7.40	3.35	4.06	2.17	10.6	12.8	8.11	2.28	5.83	0.35	3.39	1.69
½	7.40	3.35	4.06	2.17	10.6	12.8	8.11	2.28	5.83	0.63	3.39	1.69
1	7.40	3.35	4.06	2.17	10.6	12.8	8.11	2.28	5.83	1.02	3.39	2.20
1 ½	7.40	3.35	4.06	2.13	10.6	12.8	8.11	2.28	5.83	1.37	5.51	4.21
2	7.40	3.35	4.06	2.36	10.9	13.2	8.11	2.28	5.83	1.87	5.51	4.72
3	7.40	3.35	4.06	2.91	11.4	14.3	8.11	2.28	5.83	2.87	5.51	5.83
4	7.40	3.35	4.06	3.43	11.9	15.4	8.11	2.28	5.83	3.83	5.51	6.85
6	7.40	3.35	4.06	4.61	13.1	17.7	8.11	2.28	5.83	5.78	7.87	9.21


- 1) Depending on the cable gland used: values up to + 1.18 in  
 2) For version without local display: values – 1.18 in  
 3) Total length (L) depends on the process connections.

*Order code for "Housing", option B "Stainless, hygienic"*

DN [in]	A <sup>1)</sup> [in]	B <sup>1)</sup> [in]	C [in]	D [in]	E [in]	F [in]	G <sup>2)</sup> [in]	H [in]	I <sup>2)</sup> [in]	K [in]	L <sup>3)</sup> [in]	M [in]
¼	7.20	2.87	4.33	2.17	10.0	12.2	8.15	2.56	5.59	0.09	3.39	1.69
⅜	7.20	2.87	4.33	2.17	10.0	12.2	8.15	2.56	5.59	0.18	3.39	1.69
¾	7.20	2.87	4.33	2.17	10.0	12.2	8.15	2.56	5.59	0.35	3.39	1.69
½	7.20	2.87	4.33	2.17	10.0	12.2	8.15	2.56	5.59	0.63	3.39	1.69
1	7.20	2.87	4.33	2.17	10.0	12.2	8.15	2.56	5.59	1.02	3.39	2.20
1 ½	7.20	2.87	4.33	2.13	10.0	12.2	8.15	2.56	5.59	1.37	5.51	4.21
2	7.20	2.87	4.33	2.63	10.3	12.6	8.15	2.56	5.59	1.87	5.51	4.72
3	7.20	2.87	4.33	2.91	10.8	13.7	8.15	2.56	5.59	2.87	5.51	5.83
4	7.20	2.87	4.33	3.43	11.3	14.8	8.15	2.56	5.59	3.83	5.51	6.85
6	7.20	2.87	4.33	4.61	12.5	17.1	8.15	2.56	5.59	5.78	7.87	9.21


- 1) Depending on the cable gland used: values up to + 1.18 in  
 2) For version without local display: values – 1.18 in  
 3) Total length (L) depends on the process connections.

Sensor flange connection



47 Front view without process connections

DN	A	B	C	D	E	F	G	H	K	L	M
[in]	[in]	[in]	[in]	[in]	[in]	[in]	[in]	[in]	[in]	[in]	[mm]
1/12	2.44	1.64	1.34	0.35	0.94	1.65	1.69	0.33	0.24	0.16	M6
5/32	2.44	1.64	1.34	0.35	0.94	1.65	1.69	0.33	0.24	0.16	M6
5/16	2.44	1.64	1.34	0.35	0.94	1.65	1.69	0.33	0.24	0.16	M6
½	2.44	1.64	1.34	0.63	0.94	1.65	1.69	0.33	0.24	0.16	M6
1	2.83	1.98	1.73	0.89	1.14	2.17	2.20	0.33	0.24	0.16	M6



48 Front view without process connections


DN	A	B	C	D	E	F	G	H	K	L
[in]	[in]	[in]	[in]	[in]	[in]	[mm]	[in]	[in]	90° ±0.5° Tapped holes	60° ±0.5°
1 ½	3.93	3.38	2.80	1.90	1.37	M8	0.47	0.67	4	–
2	4.44	3.89	3.29	2.37	1.87	M8	0.47	0.67	4	–
3	5.54	5.26	4.49	3.50	2.87	M8	0.47	0.67	–	6
4	6.56	6.28	5.55	4.50	3.83	M8	0.47	0.67	–	6



DN	A	B	C	D	E	F	G	H	K	L
[in]	[in]	[in]	[in]	[in]	[in]	[mm]	[in]	[in]	90° ±0.5° Tapped holes	60° ±0.5°
5	7.82	7.54	6.73	5.50	4.72	M10	0.59	0.79	–	6
6	8.93	8.64	7.87	6.63	5.78	M10	0.59	0.79	–	6

Flange connections

Flanges with O-ring seal




A0015621

Flange according to ASME B16.5: Class 150 1.4404 (316L) Order code for "Process connection", option A1S						
DN [in]	A [in]	B [in]	C [in]	D [in]	E [in]	L [in]
1/12 to 3/8 <sup>1)</sup>	3.50	2.38	4 × Ø 0.62	0.44	0.62	8.59
1/2	3.50	2.38	4 × Ø 0.62	0.44	0.63	8.59
1	4.25	3.12	4 × Ø 0.62	0.56	1.05	9.05

Surface roughness: R<sub>a</sub> ≤ 63 µin

1) DN 1/12 to 3/8 with DN 1/2" flanges as standard



A0022221

**Lap joint flange according to ASME B16.5: Class 150**  
**PVDF**
*Order code for "Process connection", option A1P*

DN [in]	A [in]	B [in]	C [in]	D [in]	E [in]	F [in]	L [in]
$\frac{1}{12}$ to $\frac{3}{8}$ <sup>1)</sup>	3.74	2.36	$4 \times \varnothing 0.62$	0.59	1.38	0.63	7.87
$\frac{1}{2}$	3.74	2.36	$4 \times \varnothing 0.62$	0.59	1.38	0.63	7.87

 Surface roughness:  $R_a \leq 63 \mu\text{in}$ 

The required grounding rings can be ordered as accessories (order code: DK5HR-\*\*\*\*).

- 1) DN
- $\frac{1}{12}$
- to
- $\frac{3}{8}$
- with DN
- $\frac{1}{2}$
- " flanges as standard


**Lap joint flange according to ASME B16.5: Class 150**  
**PVDF**
*Order code for "Process connection", option A4P*

DN [in]	A [in]	B [in]	C [in]	D [in]	E [in]	F [in]	L [in]
$\frac{1}{12}$ to $\frac{3}{8}$ <sup>1)</sup>	3.74	2.36	$4 \times \varnothing 0.62$	0.59	1.38	0.63	7.87
$\frac{1}{2}$	3.74	2.36	$4 \times \varnothing 0.62$	0.59	1.38	0.63	7.87

 Surface roughness:  $R_a \leq 63 \mu\text{in}$ 

Grounding rings are not necessary.

- 1) DN
- $\frac{1}{12}$
- to
- $\frac{3}{8}$
- with DN
- $\frac{1}{2}$
- " flanges as standard

**Welding nipple**
*Welding nipple with aseptic gasket seal*


A0027510

**Welding nipple according to ISO 2037**  
**1.4404 (316L)**
*Order code for "Process connection", option IAS*

DN [in]	Suitable for pipe ISO 2037 [in]	A [in]	B [in]	L [in]
$\frac{1}{12}$ to $\frac{3}{8}$	$0.50 \times 0.06$	0.47	0.39	4.65
$\frac{1}{2}$	$0.75 \times 0.06$	0.71	0.63	4.65
1	$1.00 \times 0.06$	0.98	0.89	4.65
$1 \frac{1}{2}$	$1.50 \times 0.05$	1.50	1.40	8.66
2	$2.00 \times 0.05$	2.01	1.91	8.66
3	$3.00 \times 0.06$	3.00	2.87	8.66
4	$2.50 \times 0.08$	4.00	3.84	8.66
5	$4.00 \times 0.08$	5.50	5.34	15.00

**Welding nipple according to ISO 2037**  
**1.4404 (316L)**
*Order code for "Process connection", option IAS*

DN [in]	Suitable for pipe ISO 2037 [in]	A [in]	B [in]	L [in]
6	6.63 × 0.10	6.63	6.42	15.00

 Surface roughness:  $R_a \leq 31.5 \mu\text{in}$ , optional  $\leq 15 \mu\text{in}$ 


Please note the internal diameters of the measuring tube and process connection (B) when cleaning with pigs.

**Welding nipple according to ASME BPE**
**1.4404 (316L)**
*Order code for "Process connection", option AAS*

DN [in]	Suitable for pipe ASME BPE [in]	A [in]	B [in]	L [in]
$\frac{1}{12}$ to $\frac{3}{8}$	0.50 × 0.06	0.50	0.35	4.65
$\frac{1}{2}$	0.75 × 0.06	0.75	0.63	4.65
1	1.00 × 0.06	1.00	0.89	4.65
1 $\frac{1}{2}$	1.50 × 0.06	1.50	1.37	8.66
2	2.00 × 0.06	2.00	1.87	8.66
3	3.00 × 0.06	3.00	2.87	8.66
4	4.00 × 0.08	4.00	3.83	8.66
6	6.00 × 0.11	6.00	5.90	11.80

 Surface roughness:  $R_a \leq 31.5 \mu\text{in}$ , optional  $\leq 15 \mu\text{in}$ 

Please note the internal diameters of the measuring tube and process connection (B) when cleaning with pigs.

**Welding nipple with O-ring seal**


A0027510


**Welding nipple according to ODT/SMS**
**1.4404 (316L)**
*Order code for "Process connection", option A2S*

DN [in]	Suitable for pipe ODT/SMS [in]	A [in]	B [in]	L [in]
$\frac{1}{12}$ to $\frac{3}{8}$	0.53 × 0.09	0.53	0.35	4.99
$\frac{1}{2}$	0.84 × 0.10	0.84	0.63	4.99

 Surface roughness:  $R_a \leq 63 \mu\text{in}$

## Clamp connections

*Clamp connections with aseptic gasket seal*



A0015625

### Tri-Clamp 1.4404 (316L)

Order code for "Process connection", option FAS

DN [in]	Suitable for pipe as per ASME BPE [in]	A [in]	B [in]	L [in]
$\frac{1}{12}$ to $\frac{3}{8}$	$\frac{1}{2}$	1	0.37	5.63
$\frac{1}{2}$	$\frac{3}{4}$	25	0.62	5.63
1	1	2	0.87	5.63
1 $\frac{1}{2}$	$1.50 \times 0.06$	1.98	1.37	8.66
2	$2.00 \times 0.06$	2.52	1.87	8.66
3	$3.00 \times 0.06$	3.58	2.87	8.66
4	$4.00 \times 0.08$	4.68	3.83	8.66
6	$6.00 \times 0.11$	6.57	5.90	11.80

Surface roughness:  $R_a \leq 31.5 \mu\text{m}$ , optional  $\leq 15 \mu\text{m}$

Please note the internal diameters of the measuring tube and process connection (B) when cleaning with pigs.


### Clamp according to ISO 2852, Fig. 2 1.4404 (316L)

Order code for "Process connection", option IBS

DN [in]	Suitable for pipe ISO 2037 [in]	DN Clamp ISO 2852 [in]	A [in]	B [in]	L [in]
1	$0.96 \times 0.06$	1	2.00	0.89	6.87
1 $\frac{1}{2}$	$1.50 \times 0.06$	1.50	1.99	1.40	8.66
2	$2.00 \times 0.06$	2.01	2.52	1.91	8.66
3	$3.00 \times 0.06$	3.00	3.58	2.87	8.66
4	$2.50 \times 0.08$	4.00	4.69	3.84	8.66
5	$4.00 \times 0.08$	5.50	6.10	5.34	11.80
6	$6.63 \times 0.10$	6.63	7.20	6.42	11.80

Surface roughness:  $R_a \leq 31.5 \mu\text{m}$ , optional  $\leq 15 \mu\text{m}$

Please note the internal diameters of the measuring tube and process connection (B) when cleaning with pigs.

**Threaded glands***Thread with aseptic gasket seal*

A0027509

**Coupling SC DIN 11851, thread  
1.4404 (316L)***Order code for "Process connection", option DCS*

DN [in]	Suitable for pipe EN 10357 (DIN 11850) [in]	A [in]	B [in]	L [in]
½	Pipe ODT ¾	Rd 0.05 × 0.13	0.63	6.85
1 ½	1.65 × 0.06	Rd 2.56 × 1/6	1.50	10.20
2	2.13 × 0.06	Rd 3.07 × 1/6	1.97	10.20
3	3.35 × 0.08	Rd 4.33 × 1/4	3.19	11.00
4	4.09 × 0.08	Rd 5.12 × 1/4	3.94	11.40
5	5.08 × 0.08	Rd 6.30 × 1/4	4.92	15.00
6	6.06 × 0.08	Rd 6.30 × 1/4	5.91	15.40

Surface roughness:  $R_a \leq 31.5 \mu\text{in}$ , optional  $\leq 15 \mu\text{in}$ 

Please note the internal diameters of the measuring tube and process connection (B) when cleaning with pigs.

**Coupling ISO 2853, thread  
1.4404 (316L)***Order code for "Process connection", option ICS*

DN [in]	Suitable for pipe EN 10357 (DIN 11850) [in]	DN Clamp ISO 2853 [in]	A [in]	B [in]	L [in]
1 ½	1.50 × 0.06	1.50	Tr 2.00 × 0.13	1.40	10.80
2	2.00 × 0.06	2.01	Tr 2.52 × 0.13	1.91	10.80
3	3.00 × 0.06	3.00	Tr 3.58 × 0.13	2.87	10.90
4	2.50 × 0.08	4.00	Tr 4.65 × 0.13	3.84	11.30

Surface roughness:  $R_a \leq 31.5 \mu\text{in}$ , optional  $\leq 15 \mu\text{in}$ 

Please note the internal diameters of the measuring tube and process connection (B) when cleaning with pigs.

**Coupling SMS 1145, thread  
1.4404 (316L)***Order code for "Process connection", option SAS*


DN [in]	Suitable for pipe ODT [in]	DN SMS 1145 [in]	A [in]	B [in]	L [in]
1	1	1	Rd 1.57 × 0.17	0.89	5.81
1 ½	1.50 × 0.06	1.50	Rd 2.36 × 1/6	1.37	10.10
2	2.00 × 0.06	2.00	Rd 2.76 × 1/6	1.87	10.10

**Coupling SMS 1145, thread  
1.4404 (316L)**
*Order code for "Process connection", option SAS*

DN [in]	Suitable for pipe ODT [in]	DN SMS 1145 [in]	A [in]	B [in]	L [in]
3	3.00 × 0.06	3.00	Rd 3.86 × 1/6	2.86	10.90
4	4.00 × 0.08	4.00	Rd 5.20 × 1/6	3.83	11.30

 Surface roughness:  $R_a \leq 31.5 \mu\text{in}$ , optional  $\leq 15 \mu\text{in}$ 

Please note the internal diameters of the measuring tube and process connection (B) when cleaning with pigs.

**Thread with O-ring seal**


A0027509

**External thread according to ISO 228/DIN 2999  
1.4404 (316L)**
*Order code for "Process connection", option I2S*

DN [in]	Suitable for internal thread ISO 228 / DIN 2999 [in]	A [in]	B [in]	L [in]
$\frac{1}{12}$ to $\frac{3}{8}$	R 3/8	Rd 0.40 × 3/8	0.39	6.53
$\frac{1}{2}$	R 1/2	Rd 0.52 × 1/2	0.63	6.53
1	R 1	Rd 0.66 × 1	0.98	6.69


 Surface roughness:  $R_a \leq 63 \mu\text{in}$ 
**Internal thread according to ISO 228/DIN 2999  
1.4404 (316L)**
*Order code for "Process connection", option I3S*

DN [in]	Suitable for external thread ISO 228 / DIN 2999 [in]	A [in]	B [in]	L [in]
$\frac{1}{12}$ to $\frac{3}{8}$	Rp 3/8	Rd 0.51 × 3/8	0.35	6.93
$\frac{1}{2}$	Rp 1/2	Rd 0.55 × 1/2	0.63	6.93
1	Rp 1	Rd 0.67 × 1	1.07	7.41

 Surface roughness:  $R_a \leq 63 \mu\text{in}$

Adhesive sleeves

Adhesive sleeves with O-ring seal




A0027510

Adhesive sleeve PVC				
Order code for "Process connection", options O1V, O2V				
DN [in]	Suitable for pipe [in]	A [in]	B [in]	L [in]
$\frac{1}{12}$ to $\frac{3}{8}$	$\frac{1}{2}$	1.07	0.85	6.43
Surface roughness: $R_a \leq 63 \mu\text{in}$ The required grounding rings can be ordered as accessories (order code: DK5HR-****).				

Mounting kits

Wall mounting kit




A0005537


A [in]	B [in]	C [in]	Ø D [in]	E [in]	F [in]
5.39	4.33	4.72	0.28	4.92	3.46

Accessories

Protective cover




Remote display and operating module DKX001



49 Engineering unit mm (in)

External WLAN antenna

External WLAN antenna mounted on device




50 Engineering unit mm (in)



External WLAN antenna mounted with cable


The external WLAN antenna can be mounted separately from the transmitter if the transmission/reception conditions at the transmitter mounting location are poor.



A0033597

51 Engineering unit mm (in)


Spacer



A0017294

Order code: DK5HB-****				
DN [in]	di [in]	D1 [in]	D2 [in]	L [in]
3	2.87	5.54	5.55	1.30
4	3.83	6.56	6.38	1.30

Clamp connections with aseptic gasket seal available for order



A0015625


52 Hygienic clamp adapter connection suitable for pipes with connection according to ASME BPE (reduction)

**Tri-Clamp****1.4404 (316L)****Order code: DKH\*\*-HF\*\***

DN [in]	Suitable for pipe in accordance with ASME BPE (reduction) [in]	A [in]	B [in]	L [in]
½	Pipe ODT 1	2	0.87	5.63

Surface roughness:  $R_a \leq 31.5 \mu\text{in}$ , optional  $\leq 15 \mu\text{in}$   
Please note the internal diameters of the measuring tube and process connection (B) when cleaning with pigs.

*Threaded glands with O-ring seal available for order*



A0027509

**External thread****1.4404 (316L)****Order code: DKH\*\*-GD\*\***

DN [in]	Suitable for NPT internal thread [in]	A [in]	B [in]	L [in]
1/12 to 3/8	NPT 3/8	R 0.61 × 3/8	0.39	7.39
½	NPT ½	R 0.79 × ½	0.63	7.39
1	NPT 1	R 1 × 1	1.00	7.73


Surface roughness:  $R_a \leq 63 \mu\text{in}$

**Internal thread****1.4404 (316L)****Order code: DKH\*\*-GC\*\***

DN [in]	Suitable for NPT external thread [in]	A [in]	B [in]	L [in]
1/12 to 3/8	NPT 3/8	R 0.51 × 3/8	0.35	6.93
½	NPT ½	R 0.55 × ½	0.63	6.93
1	NPT 1	R 0.67 × 1	1.07	7.41

Surface roughness:  $R_a \leq 63 \mu\text{in}$

## Grounding rings



A0017673

For lap joint flange made of PVDF and PVC adhesive sleeve  
 1.4435 (316L), Alloy C22, tantalum  
 Order code: DK5HR-\*\*\*\*

DN [in]	di [in]	B [in]	C [in]	D [in]	E [in]	F [in]	G [in]	H [in]	J [in]
$\frac{1}{12}$ to $\frac{3}{8}$	0.35	0.87	0.69	1.33	0.02	0.14	0.07	0.13	0.18
$\frac{1}{2}$	0.63	1.14	0.97	1.33	0.02	0.14	0.07	0.13	0.18
1	0.89	1.44	1.23	1.73	0.02	0.14	0.07	0.13	0.18

## Weight

All values (weight exclusive of packaging material) refer to devices for standard pressure ratings. Weight specifications including transmitter as per order code for "Housing", option A "Aluminum, coated".

Different values due to different transmitter versions:

- Transmitter version for the hazardous area  
(Order code for "Housing", option A "Aluminum, coated"; Ex d): +2 kg (+4.4 lbs)
- Transmitter version for hygienic area  
(Order code for "Housing", option B "Stainless, hygienic"): +0.2 kg (+0.44 lbs)

Nominal diameter		Weight	
[mm]	[in]	[kg]	[lbs]
2	1/12	4.7	10.4
4	5/32	4.7	10.4
8	5/16	4.7	10.4
15	$\frac{1}{2}$	4.6	10.1
25	1	5.5	12.1
40	1 $\frac{1}{2}$	6.8	15.0
50	2	7.3	16.1
65	–	8.1	17.9
80	3	8.7	19.2
100	4	10.0	22.1
125	5	15.4	34.0
150	6	17.8	39.3

Measuring tube specification

Nominal diameter		Pressure rating <sup>1)</sup>	Process connection internal diameter	
		EN (DIN)	PFA	
[mm]	[in]	[bar]	[mm]	[in]
2	1/12	PN 16/40	2.25	0.09
4	5/32	PN 16/40	4.5	0.18
8	5/16	PN 16/40	9.0	0.35
15	½	PN 16/40	16.0	0.63
–	1	PN 16/40	22.6	0.89
25	–	PN 16/40	26.0	1.02

1) Depending on process connection and seals used

Materials

Transmitter housing

- Order code for "Housing":
- Option **A** "Aluminum, coated": aluminum, AlSi10Mg, coated
  - Option **B** "Stainless, hygienic": stainless steel, 1.4404 (316L)


Window material

- Order code for "Housing":
- Option **A** "Aluminum, coated": glass
  - Option **B** "Stainless, hygienic": polycarbonate
- For order code for "Approval", option **BS, CZ, GS, MS** and **NS**: glass

Seals

- Order code for "Housing":
- Option **B** "Stainless, hygienic": EPDM

Cable entries/cable glands



A0028352

53 Possible cable entries/cable glands

- 1 Female thread M20 × 1.5
- 2 Cable gland M20 × 1.5
- 3 Adapter for cable entry with internal thread G ½" or NPT ½"
- 4 Device plug connectors

Order code for "Housing", option A "Aluminum, coated"

The various cable entries are suitable for hazardous and non-hazardous areas.

Cable entry/cable gland	Material
Cable gland M20 × 1.5	Plastic/nickel-plated brass
Adapter for cable entry with internal thread G ½"	Nickel-plated brass

Cable entry/cable gland	Material
Adapter for cable entry with internal thread NPT ½"	
Device plug connectors	Plug M12 × 1 <ul style="list-style-type: none"> <li>▪ Socket: Stainless steel, 1.4404 (316L)</li> <li>▪ Contact housing: Polyamide</li> <li>▪ Contacts: Gold-plated brass</li> </ul>

**Device plug**

Electrical connection	Material
Plug M12x1	<ul style="list-style-type: none"> <li>▪ Socket: Stainless steel, 1.4404 (316L)</li> <li>▪ Contact housing: Polyamide</li> <li>▪ Contacts: Gold-plated brass</li> </ul>

**Sensor housing**

Stainless steel 1.4301 (304)

**Measuring tubes**

Stainless steel 1.4301 (304)

*Liner*

PFA (USP Class VI, FDA 21 CFR 177.1550, 3A)

**Process connections**

- Stainless steel, 1.4404 (F316L)
- PVDF
- PVC adhesive sleeve

**Electrodes**

Standard: 1.4435 (316L)

**Seals**

- O-ring seal, DN 2 to 25 (1/12 to 1"): EPDM, FKM, Kalrez
- Aseptic gasket seal, DN 2 to 150 (1/12 to 6"): EPDM <sup>1)</sup>, FKM, silicone <sup>1)</sup>

**Accessories***Protective cover*

Stainless steel, 1.4404 (316L)

*External WLAN antenna*

- Antenna: ASA plastic (acrylic ester-styrene-acrylonitrile) and nickel-plated brass
- Adapter: Stainless steel and nickel-plated brass
- Cable: Polyethylene
- Plug: Nickel-plated brass
- Angle bracket: Stainless steel

*Grounding rings*

- Standard: 1.4435 (316L)
- Optional: Alloy C22, tantalum

*Wall mounting kit*



Stainless steel 1.4301 (304)

---



1) USP Class VI, FDA 21 CFR 177.2600, 3A

*Spacer*

1.4435 (F316L)

<b>Fitted electrodes</b>	<ul style="list-style-type: none"> <li>■ 2 measuring electrodes for signal detection</li> <li>■ 1 empty pipe detection electrode for empty pipe detection/temperature measurement (only DN 15 to 150 (½ to 6"))</li> </ul>
<b>Process connections</b>	<p>With O-ring seal:</p> <ul style="list-style-type: none"> <li>■ Welding nipple (DIN EN ISO 1127, ODT/SMS, ISO 2037)</li> <li>■ Flange (EN (DIN), ASME, JIS)</li> <li>■ Flange from PVDF (EN (DIN), ASME, JIS)</li> <li>■ External thread</li> <li>■ Internal thread</li> <li>■ Hose connection</li> <li>■ PVC adhesive sleeve</li> </ul> <p>With aseptic molded seal:</p> <ul style="list-style-type: none"> <li>■ Coupling (DIN 11851, DIN 11864-1, ISO 2853, SMS 1145)</li> <li>■ Flange DIN 11864-2</li> </ul> <p> For information on the different materials used in the process connections →  89</p>
<b>Surface roughness</b>	<p>Stainless steel electrodes, 1.4435 (316L); Alloy C22, 2.4602 (UNS N06022); platinum; tantalum:  <math>\leq 0.3</math> to <math>0.5\ \mu\text{m}</math> (11.8 to <math>19.7\ \mu\text{in}</math>)          (All data relate to parts in contact with fluid)</p> <p>Liner with PFA:  <math>\leq 0.4\ \mu\text{m}</math> (<math>15.7\ \mu\text{in}</math>)          (All data relate to parts in contact with fluid)</p> <p>Stainless steel process connections:</p> <ul style="list-style-type: none"> <li>■ With O-ring seal: <math>\leq 1.6\ \mu\text{m}</math> (<math>63\ \mu\text{in}</math>)</li> <li>■ With aseptic seal: <math>\leq 0.8\ \mu\text{m}</math> (<math>31.5\ \mu\text{in}</math>)</li> <li>Optional: <math>\leq 0.38\ \mu\text{m}</math> (<math>15\ \mu\text{in}</math>)</li> </ul> <p>(All data relate to parts in contact with fluid)</p>

## Operability

<b>Operating concept</b>	<p><b>Operator-oriented menu structure for user-specific tasks</b></p> <ul style="list-style-type: none"> <li>■ Commissioning</li> <li>■ Operation</li> <li>■ Diagnostics</li> <li>■ Expert level</li> </ul> <p><b>Fast and safe commissioning</b></p> <ul style="list-style-type: none"> <li>■ Guided menus ("Make-it-run" wizards) for applications</li> <li>■ Menu guidance with brief descriptions of the individual parameter functions</li> <li>■ Device access via Web server or SmartBlue app →  108</li> <li>■ WLAN access to the device via mobile handheld terminal, tablet or smart phone</li> </ul> <p><b>Reliable operation</b></p> <ul style="list-style-type: none"> <li>■ Operation in local language →  91</li> <li>■ Uniform operating philosophy applied to device and operating tools</li> <li>■ If replacing electronic modules, transfer the device configuration via the integrated memory (HistoROM backup) which contains the process and measuring device data and the event logbook. No need to reconfigure.</li> </ul> <p><b>Efficient diagnostics increase measurement availability</b></p> <ul style="list-style-type: none"> <li>■ Troubleshooting measures can be called up via the device and in the operating tools</li> <li>■ Diverse simulation options, logbook for events that occur and optional line recorder functions</li> </ul>
--------------------------	---

**Languages**

Can be operated in the following languages:

- Via local operation  
English, German, French, Spanish, Italian, Dutch, Portuguese, Polish, Russian, Turkish, Chinese, Japanese, Korean, Bahasa (Indonesian), Vietnamese, Czech, Swedish
- Via Web browser  
English, German, French, Spanish, Italian, Dutch, Portuguese, Polish, Russian, Turkish, Chinese, Japanese, Korean, Bahasa (Indonesian), Vietnamese, Czech, Swedish
- Via "FieldCare", "DeviceCare" operating tool: English, German, French, Spanish, Italian, Chinese, Japanese


**Local operation****Via display module**

Two display modules are available:

- Order code for "Display; operation", option **F** "4-line, illuminated, graphic display; touch control"
- Order code for "Display; operation", option **G** "4-line, illuminated, graphic display; touch control + WLAN"



Information about WLAN interface → 97



A0026785

54 Operation with touch control

*Display elements*

- 4-line, illuminated, graphic display
- White background lighting; switches to red in event of device errors
- Format for displaying measured variables and status variables can be individually configured
- Permitted ambient temperature for the display: -20 to +60 °C (-4 to +140 °F)  
The readability of the display may be impaired at temperatures outside the temperature range.


*Operating elements*

- External operation via touch control (3 optical keys) without opening the housing: ⊕, □, ⊞
- Operating elements also accessible in the various zones of the hazardous area

**Via remote display and operating module DKX001**

The remote display and operating module DKX001 is available as an optional extra → 106.

- The remote display and operating module DKX001 is only available for the following housing version: order code for "Housing": option A "Aluminum, coated"
- The measuring device is always supplied with a dummy cover when the remote display and operating module DKX001 is ordered directly with the measuring device. Display or operation at the transmitter is not possible in this case.
- If ordered subsequently, the remote display and operating module DKX001 may not be connected at the same time as the existing measuring device display module. Only one display or operation unit may be connected to the transmitter at any one time.



A0026786

55 Operation via remote display and operating module DKX001

Display and operating elements

The display and operating elements correspond to those of the display module .

Material

The housing material of the display and operating module DKX001 corresponds to the selected material of the transmitter housing.

Transmitter housing		Remote display and operating module
Order code for "Housing"	Material	Material
Option A "Aluminum, coated"	AlSi10Mg, coated	AlSi10Mg, coated

Cable entry

Corresponds to the choice of transmitter housing, order code for "Electrical connection".

Connecting cable

→ 40

Dimensions


→ 71

Remote operation

Via HART protocol

This communication interface is available in device versions with a HART output.






A0028747

56 Options for remote operation via HART protocol (active)

- 1 Control system (e.g. PLC)
- 2 Field Communicator 475
- 3 Computer with Web browser (e.g. Internet Explorer) for accessing the integrated device Web server or computer with operating tool (e.g. FieldCare, DeviceCare, AMS Device Manager, SIMATIC PDM) with COM DTM "CDI Communication TCP/IP"
- 4 Commubox FXA195 (USB)
- 5 Field Xpert SFX350 or SFX370
- 6 VIATOR Bluetooth modem with connecting cable
- 7 Transmitter




A0028746

57 Options for remote operation via HART protocol (passive)

- 1 Control system (e.g. PLC)
- 2 Transmitter power supply unit, e.g. RN221N (with communication resistor)
- 3 Connection for Commubox FXA195 and Field Communicator 475
- 4 Field Communicator 475
- 5 Computer with Web browser (e.g. Internet Explorer) for accessing the integrated device Web server or computer with operating tool (e.g. FieldCare, DeviceCare, AMS Device Manager, SIMATIC PDM) with COM DTM "CDI Communication TCP/IP"
- 6 Commubox FXA195 (USB)
- 7 Field Xpert SFX350 or SFX370
- 8 VIATOR Bluetooth modem with connecting cable
- 9 Transmitter

### Via FOUNDATION Fieldbus network

This communication interface is available in device versions with FOUNDATION Fieldbus.




A0028837

58 Options for remote operation via FOUNDATION Fieldbus network

- 1 Automation system
- 2 Computer with FOUNDATION Fieldbus network card
- 3 Industry network
- 4 High Speed Ethernet FF-HSE network
- 5 Segment coupler FF-HSE/FF-H1
- 6 FOUNDATION Fieldbus FF-H1 network
- 7 Power supply FF-H1 network
- 8 T-box
- 9 Measuring device

#### Via PROFIBUS PA network

This communication interface is available in device versions with PROFIBUS PA.




A0028838

59 Options for remote operation via PROFIBUS PA network

- 1 Automation system
- 2 Computer with PROFIBUS network card
- 3 PROFIBUS DP network
- 4 Segment coupler PROFIBUS DP/PA
- 5 PROFIBUS PA network
- 6 T-box
- 7 Measuring device

### Via Modbus RS485 protocol

This communication interface is available in device versions with a Modbus-RS485 output.



A0029437


60 Options for remote operation via Modbus-RS485 protocol (active)

- 1 Control system (e.g. PLC)
- 2 Computer with Web browser (e.g. Internet Explorer) for accessing the integrated device Web server or with operating tool (e.g. FieldCare, DeviceCare) with COM DTM "CDI Communication TCP/IP" or Modbus DTM
- 3 Transmitter

### Via EtherNet/IP network

This communication interface is available in device versions with EtherNet/IP.

#### Star topology




A0032078

61 Options for remote operation via EtherNet/IP network: star topology

- 1 Automation system, e.g. "RSLogix" (Rockwell Automation)
- 2 Workstation for measuring device operation: with Custom Add-On Profile for "RSLogix 5000" (Rockwell Automation) or with Electronic Data Sheet (EDS)
- 3 Computer with Web browser (e.g. Internet Explorer) for accessing the integrated device Web server or computer with operating tool (e.g. FieldCare, DeviceCare) with COM DTM "CDI Communication TCP/IP"
- 4 Ethernet switch
- 5 Measuring device

#### Ring topology

The device is integrated via the terminal connection for signal transmission (output 1) and the service interface (CDI-RJ45).



A0033725


62 Options for remote operation via EtherNet/IP network: ring topology

- 1 Automation system, e.g. "RSLogix" (Rockwell Automation)
- 2 Workstation for measuring device operation: with Custom Add-On Profile for "RSLogix 5000" (Rockwell Automation) or with Electronic Data Sheet (EDS)
- 3 Computer with Web browser (e.g. Internet Explorer) for accessing the integrated device Web server or computer with operating tool (e.g. FieldCare, DeviceCare) with COM DTM "CDI Communication TCP/IP"
- 4 Ethernet switch
- 5 Measuring device

### Via PROFINET network

This communication interface is available in device versions with PROFINET.

#### Star topology




A0026545

63 Options for remote operation via PROFINET network: star topology

- 1 Automation system, e.g. Simatic S7 (Siemens)
- 2 Computer with Web browser (e.g. Internet Explorer) for accessing the integrated device Web server or computer with operating tool (e.g. FieldCare, DeviceCare, SIMATIC PDM) with COM DTM "CDI Communication TCP/IP"
- 3 Switch, e.g. Scalance X204 (Siemens)
- 4 Measuring device

#### Ring topology

This communication interface is available in device versions with PROFINET.



A0033719

64 Options for remote operation via PROFINET network: ring topology

- 1 Automation system, e.g. Simatic S7 (Siemens)
- 2 Computer with Web browser (e.g. Internet Explorer) for accessing the integrated device Web server or computer with operating tool (e.g. FieldCare, DeviceCare, SIMATIC PDM) with COM DTM "CDI Communication TCP/IP"
- 3 Switch, e.g. Scalance X204 (Siemens)
- 4 Measuring device

## Service interface


### Via service interface (CDI-RJ45)

A point-to-point connection can be established to configure the device onsite. With the housing open, the connection is established directly via the service interface (CDI-RJ45) of the device.



An adapter for RJ45 and the M12 connector is optionally available:  
Order code for "Accessories", option **NB**: "Adapter RJ45 M12 (service interface)"

The adapter connects the service interface (CDI-RJ45) to an M12 connector mounted in the cable entry. Therefore the connection to the service interface can be established via an M12 connector without opening the device.



A0027563


65 Connection via service interface (CDI-RJ45)

- 1 Computer with Web browser (e.g. Microsoft Internet Explorer, Microsoft Edge) for accessing the integrated device Web server or with "FieldCare", "DeviceCare" operating tool with COM DTM "CDI Communication TCP/IP" or Modbus DTM
- 2 Standard Ethernet connecting cable with RJ45 connector
- 3 Service interface (CDI-RJ45) of the measuring device with access to the integrated Web server

### Via WLAN interface


The optional WLAN interface is available on the following device version:

Order code for "Display; operation", option **G** "4-line, illuminated, graphic display; touch control + WLAN"



A0034570


- 1 Transmitter with integrated WLAN antenna
- 2 Transmitter with external WLAN antenna
- 3 LED lit constantly: WLAN reception is enabled on measuring device
- 4 LED flashing: WLAN connection established between operating unit and measuring device
- 5 Computer with WLAN interface and Web browser (e.g. Microsoft Internet Explorer, Microsoft Edge) for accessing the integrated device Web server or with operating tool (e.g. FieldCare, DeviceCare)
- 6 Mobile handheld terminal with WLAN interface and Web browser (e.g. Microsoft Internet Explorer, Microsoft Edge) for accessing the integrated device Web server or operating tool (e.g. FieldCare, DeviceCare)
- 7 Smartphone or tablet

Function	WLAN: IEEE 802.11 b/g (2.4 GHz) <ul style="list-style-type: none"> <li>Access point with DHCP server (default setting)</li> <li>Network</li> </ul>
Encryption	WPA2-PSK/AES 128 bit
Configurable WLAN channels	1 to 11
Degree of protection	IP67
Available antennas	<ul style="list-style-type: none"> <li>Internal antenna</li> <li>External antenna (optional)</li> </ul> In the event of poor transmission/reception conditions at the place of installation. Available as an accessory → 106.  Only one antenna active in each case!
Max. range	50 m (164 ft)
Materials: External WLAN antenna	<ul style="list-style-type: none"> <li>Antenna: ASA plastic (acrylic ester-styrene-acrylonitrile) and nickel-plated brass</li> <li>Adapter: Stainless steel and nickel-plated brass</li> <li>Cable: Polyethylene</li> <li>Connector: Nickel-plated brass</li> <li>Angle bracket: Stainless steel</li> </ul>




## Network integration

With the optional OPC-UA-Server application package, the device can be integrated into an Ethernet network via the service interface (CDI-RJ45 and WLAN) and communicate with OPC-UA clients. If the device is used in this way, IT security must be considered.

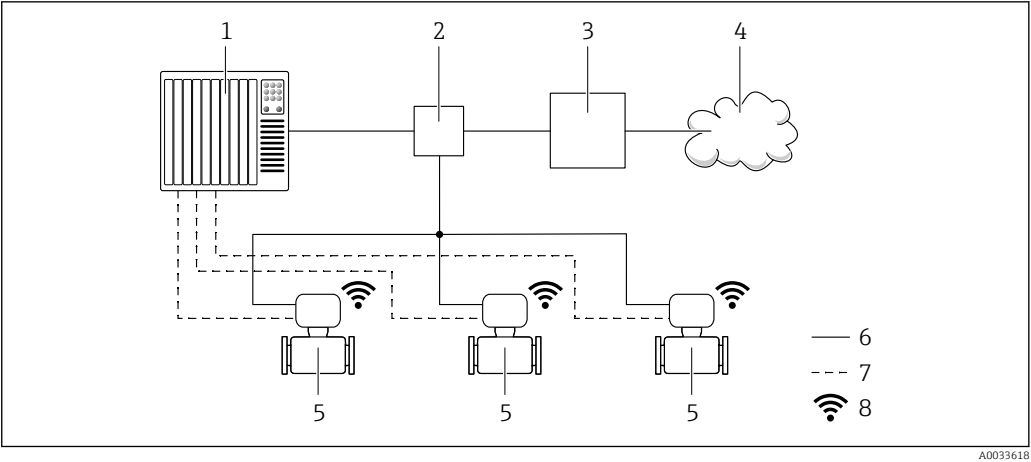
For permanent access to device data and for device configuration via the Web server, the device is incorporated directly in a network via the service interface (CDI-RJ45). In this way, the device can be accessed any time from the control station. The measured values are processed separately via the inputs and outputs through the automation system.





- 1 Automation system, e.g. Simatic S7 (Siemens)
- 2 Ethernet switch
- 3 Edge Gateway
- 4 Cloud
- 5 Measuring device
- 6 Ethernet network
- 7 Measured values via inputs and outputs
- 8 Optional WLAN interface

-  The optional WLAN interface is available on the following device version:  
Order code for "Display; operation", option **G** "4-line, illuminated, graphic display; touch control + WLAN"
-  Special Documentation for the OPC-UA-Server application package →  110.

**Supported operating tools** Different operating tools can be used for local or remote access to the measuring device. Depending on the operating tool used, access is possible with different operating units and via a variety of interfaces.

Supported operating tools	Operating unit	Interface	Additional information
Web browser	Notebook, PC or tablet with Web browser	<ul style="list-style-type: none"><li>■ CDI-RJ45 service interface</li><li>■ WLAN interface</li><li>■ Ethernet-based fieldbus (EtherNet/IP, PROFINET)</li></ul>	Special Documentation for device
DeviceCare SFE100	Notebook, PC or tablet with Microsoft Windows system	<ul style="list-style-type: none"><li>■ CDI-RJ45 service interface</li><li>■ WLAN interface</li><li>■ Fieldbus protocol</li></ul>	→  108

Supported operating tools	Operating unit	Interface	Additional information
FieldCare SFE500	Notebook, PC or tablet with Microsoft Windows system	<ul style="list-style-type: none"> <li>■ CDI-RJ45 service interface</li> <li>■ WLAN interface</li> <li>■ Fieldbus protocol</li> </ul>	→  108
Device Xpert	Field Xpert SFX 100/350/370	HART and FOUNDATION Fieldbus fieldbus protocol	Operating Instructions BA01202S Device description files: Use update function of handheld terminal

 Other operating tools based on FDT technology with a device driver such as DTM/iDTM or DD/EDD can be used for device operation. These operating tools are available from the individual manufacturers. Integration into the following operating tools, among others, is supported:

- FactoryTalk AssetCentre (FTAC) by Rockwell Automation → [www.rockwellautomation.com](http://www.rockwellautomation.com)
- Process Device Manager (PDM) by Siemens → [www.siemens.com](http://www.siemens.com)
- Asset Management Solutions (AMS) by Emerson → [www.emersonprocess.com](http://www.emersonprocess.com)
- FieldCommunicator 375/475 by Emerson → [www.emersonprocess.com](http://www.emersonprocess.com)
- Field Device Manager (FDM) by Honeywell → [www.honeywellprocess.com](http://www.honeywellprocess.com)
- FieldMate by Yokogawa → [www.yokogawa.com](http://www.yokogawa.com)
- PACTWare → [www.pactware.com](http://www.pactware.com)

The associated device description files are available at: [www.endress.com](http://www.endress.com) → Downloads


### Web server


Thanks to the integrated Web server, the device can be operated and configured via a Web browser and via a service interface (CDI-RJ45) or via a WLAN interface. The structure of the operating menu is the same as for the local display. In addition to the measured values, status information on the device is also displayed and allows the user to monitor the status of the device. Furthermore the device data can be managed and the network parameters can be configured.

A device that has a WLAN interface (can be ordered as an option) is required for the WLAN connection: order code for "Display; operation", option **G** "4-line, illuminated; touch control + WLAN". The device acts as an Access Point and enables communication by computer or a mobile handheld terminal.

### Supported functions


Data exchange between the operating unit (such as a notebook for example) and the measuring device:

- Upload the configuration from the measuring device (XML format, configuration backup)
- Save the configuration to the measuring device (XML format, restore configuration)
- Export event list (.csv file)
- Export parameter settings (.csv file or PDF file, document the measuring point configuration)
- Export the Heartbeat verification log (PDF file, only available with the "Heartbeat Verification" application package)
- Flash firmware version for device firmware upgrade, for instance
- Download driver for system integration
- Visualize up to 1000 saved measured values (only available with the **Extended HistoROM** application package →  105)

 Webserver special documentation →  110

### HistoROM data management

The measuring device features HistoROM data management. HistoROM data management comprises both the storage and import/export of key device and process data, making operation and servicing far more reliable, secure and efficient.

 When the device is delivered, the factory settings of the configuration data are stored as a backup in the device memory. This memory can be overwritten with an updated data record, for example after commissioning.



### Additional information on the data storage concept

There are different types of data storage units in which device data are stored and used by the device:

	Device memory	T-DAT	S-DAT
<b>Available data</b>	<ul style="list-style-type: none"> <li>■ Event logbook such as diagnostic events for example</li> <li>■ Parameter data record backup</li> <li>■ Device firmware package</li> <li>■ Driver for system integration for exporting via Web server, e.g.:               <ul style="list-style-type: none"> <li>– GSD for PROFIBUS PA</li> <li>– GSDXML for PROFINET</li> <li>– EDS for EtherNet/IP</li> <li>– DD for FOUNDATION Fieldbus</li> </ul> </li> </ul>	<ul style="list-style-type: none"> <li>■ Measured value logging ("Extended HistoROM" order option)</li> <li>■ Current parameter data record (used by firmware at run time)</li> <li>■ Maximum indicators (min/max values)</li> <li>■ Totalizer values</li> </ul>	<ul style="list-style-type: none"> <li>■ Sensor data: nominal diameter etc.</li> <li>■ Serial number</li> <li>■ Calibration data</li> <li>■ Device configuration (e.g. SW options, fixed I/O or multi I/O)</li> </ul>
<b>Storage location</b>	Fixed on the user interface board in the connection compartment	Attachable to the user interface board in the connection compartment	In the sensor plug in the transmitter neck part

### Data backup

#### Automatic

- The most important device data (sensor and transmitter) are automatically saved in the DAT modules
- If the transmitter or measuring device is replaced: once the T-DAT containing the previous device data has been exchanged, the new measuring device is ready for operation again immediately without any errors
- If the sensor is replaced: once the sensor has been replaced, new sensor data are transferred from the S-DAT in the measuring device and the measuring device is ready for operation again immediately without any errors
- If exchanging the electronics module (e.g. I/O electronics module): Once the electronics module has been replaced, the software of the module is compared against the current device firmware. The module software is upgraded or downgraded where necessary. The electronics module is available for use immediately afterwards and no compatibility problems occur.

#### Manual

Additional parameter data record (complete parameter settings) in the integrated device memory HistoROM backup for:

- Data backup function  
Backup and subsequent restoration of a device configuration in the device memory HistoROM backup
- Data comparison function  
Comparison of the current device configuration with the device configuration saved in the device memory HistoROM backup

### Data transfer

#### Manual

- Transfer of a device configuration to another device using the export function of the specific operating tool, e.g. with FieldCare, DeviceCare or Web server: to duplicate the configuration or to store in an archive (e.g. for backup purposes)
- Transmission of the drivers for system integration via Web server, e.g.:
  - GSD for PROFIBUS PA
  - GSDXML for PROFINET
  - EDS for EtherNet/IP
  - DD for FOUNDATION Fieldbus

### Event list

#### Automatic


- Chronological display of up to 20 event messages in the events list
- If the **Extended HistoROM** application package (order option) is enabled: up to 100 event messages are displayed in the events list along with a time stamp, plain text description and remedial measures
- The events list can be exported and displayed via a variety of interfaces and operating tools e.g. DeviceCare, FieldCare or Web server

**Data logging****Manual**

If the **Extended HistoROM** application package (order option) is enabled:

- Record up to 1 000 measured values via 1 to 4 channels
- User configurable recording interval
- Record up to 250 measured values via each of the 4 memory channels
- Export the measured value log via a variety of interfaces and operating tools e.g. FieldCare, DeviceCare or web server

## Certificates and approvals

<b>CE mark</b>	<p>The measuring system is in conformity with the statutory requirements of the applicable EU Directives. These are listed in the corresponding EU Declaration of Conformity along with the standards applied.</p> <p>Endress+Hauser confirms successful testing of the device by affixing to it the CE mark.</p>
<b>C-Tick symbol</b>	<p>The measuring system meets the EMC requirements of the "Australian Communications and Media Authority (ACMA)".</p>
<b>Ex approval</b>	<p>The measuring device is certified for use in hazardous areas and the relevant safety instructions are provided in the separate "Safety Instructions" (XA) document. Reference is made to this document on the nameplate.</p> <p> The separate Ex documentation (XA) containing all the relevant explosion protection data is available from your Endress+Hauser sales center.</p>

**ATEX, IECEX**

Currently, the following versions for use in hazardous areas are available:

*Ex db eb*

Category	Type of protection
II2G	Ex db eb ia IIC T6...T1 Gb

*Ex tb*

Category	Type of protection
II2D	Ex tb IIIC Txxx Db

*Ex ec*

Category	Type of protection
II3G	Ex ec ic IIC T5...T1 Gc

**cCSAus**

Currently, the following versions for use in hazardous areas are available:

**IS (Ex i) and XP (Ex d)**

Class I, II, III Division 1 Groups A-G

**NI (Ex nA)**

Class I Division 2 Groups A - D

**Ex de**



Class I, Zone 1 AEx/ Ex de ia IIC T6...T1 Gb



**Ex nA**

Class I, Zone 2 AEx/Ex nA ic IIC T5...T1 Gc

**Ex tb**

Zone 21 AEx/ Ex tb IIIC T\*\* °C Db

<b>Sanitary compatibility</b>	<ul style="list-style-type: none"> <li>■ 3-A approval Only devices with the order code for "Additional approval", option <b>LP</b> "3A" have 3-A approval.</li> <li>■ EHEDG-tested Only devices with the order code for "Additional approval", option <b>LT</b> "EHEDG" have been tested and meet the requirements of the EHEDG. To meet the requirements for EHEDG certification, the device must be used with process connections in accordance with the EHEDG position paper entitled "Easy Cleanable Pipe Couplings and Process Connections" (<a href="http://www.ehedg.org">www.ehedg.org</a>).</li> <li>■ FDA</li> <li>■ Food Contact Materials Regulation (EC) 1935/2004</li> <li>■ Seals FDA-compliant (apart from Kalrez seals)</li> </ul>
<b>Pharmaceutical compatibility</b>	<ul style="list-style-type: none"> <li>■ FDA</li> <li>■ USP Class VI</li> <li>■ TSE/BSE certificate of suitability</li> </ul>
<b>Functional safety</b>	<p>The measuring device can be used for flow monitoring systems (min., max., range) up to SIL 2 (single-channel architecture; order code for "Additional approval", option <b>LA</b>) and SIL 3 (multichannel architecture with homogeneous redundancy) and is independently evaluated and certified by the TÜV in accordance with IEC 61508.</p> <p>The following types of monitoring in safety equipment are possible: Volume flow</p> <p> Functional Safety Manual with information on the SIL device →  109</p>
<b>HART certification</b>	<p><b>HART interface</b></p> <p>The measuring device is certified and registered by the FieldComm Group. The measuring system meets all the requirements of the following specifications:</p> <ul style="list-style-type: none"> <li>■ Certified according to HART 7</li> <li>■ The device can also be operated with certified devices of other manufacturers (interoperability)</li> </ul>
<b>FOUNDATION Fieldbus certification</b>	<p><b>FOUNDATION Fieldbus interface</b></p> <p>The measuring device is certified and registered by the FieldComm Group. The measuring system meets all the requirements of the following specifications:</p> <ul style="list-style-type: none"> <li>■ Certified in accordance with FOUNDATION Fieldbus H1</li> <li>■ Interoperability Test Kit (ITK), revision version 6.2.0 (certificate available on request)</li> <li>■ Physical Layer Conformance Test</li> <li>■ The device can also be operated with certified devices of other manufacturers (interoperability)</li> </ul>
<b>Certification PROFIBUS</b>	<p><b>PROFIBUS interface</b></p> <p>The measuring device is certified and registered by the PNO (PROFIBUS User Organization Organization). The measuring system meets all the requirements of the following specifications:</p> <ul style="list-style-type: none"> <li>■ Certified in accordance with PROFIBUS PA Profile 3.02</li> <li>■ The device can also be operated with certified devices of other manufacturers (interoperability)</li> </ul>
<b>EtherNet/IP certification</b>	<p>The measuring device is certified and registered by the ODVA (Open Device Vendor Association). The measuring system meets all the requirements of the following specifications:</p> <ul style="list-style-type: none"> <li>■ Certified in accordance with the ODVA Conformance Test</li> <li>■ EtherNet/IP Performance Test</li> <li>■ EtherNet/IP PlugFest compliance</li> <li>■ The device can also be operated with certified devices of other manufacturers (interoperability)</li> </ul>

<b>Certification PROFINET</b>	<p><b>PROFINET interface</b></p> <p>The measuring device is certified and registered by the PNO (PROFIBUS User Organization Organization). The measuring system meets all the requirements of the following specifications:</p> <ul style="list-style-type: none"> <li>■ Certified according to: <ul style="list-style-type: none"> <li>– Test specification for PROFINET devices</li> <li>– PROFINET Security Level 2 – Netload Class</li> </ul> </li> <li>■ The device can also be operated with certified devices of other manufacturers (interoperability)</li> </ul>
<b>Radio approval</b>	<p>The measuring device has radio approval.</p> <p> For detailed information on the radio approval, see the Special Documentation</p>
<b>Pressure Equipment Directive</b>	<p>The devices can be ordered with or without a PED approval. If a device with a PED approval is required, this must be explicitly stated in the order. For devices with nominal diameters less than or equal to DN 25 (1"), this is neither possible nor necessary.</p> <ul style="list-style-type: none"> <li>■ With the identification PED/G1/x (x = category) on the sensor nameplate, Endress+Hauser confirms conformity with the "Essential Safety Requirements" specified in Appendix I of the Pressure Equipment Directive 2014/68/EC.</li> <li>■ Devices bearing this marking (PED) are suitable for the following types of medium: Media in Group 1 and 2 with a vapor pressure greater than, or smaller and equal to 0.5 bar (7.3 psi)</li> <li>■ Devices not bearing this marking (PED) are designed and manufactured according to good engineering practice. They meet the requirements of Art. 4, Par. 3 of the Pressure Equipment Directive 2014/68/EU. The range of application is indicated in tables 6 to 9 in Annex II of the Pressure Equipment Directive 2014/68/EC.</li> </ul>
<b>Measuring instrument approval</b>	<p>The measuring device is qualified to OIML R117 and has an OIML Certificate of Conformity (optional).</p>
<b>Additional certification</b>	<p><b>PWIS-free</b></p> <p>PWIS = paint-wetting impairment substances</p> <p>Order code for "Service":</p> <ul style="list-style-type: none"> <li>■ Option <b>HC</b>: PWIS-free (version A)</li> <li>■ Option <b>HD</b>: PWIS-free (version B)</li> <li>■ Option <b>HE</b>: PWIS-free (version C)</li> </ul> <p> For more information on PWIS-free certification, see "Test specification" document TS01028D</p>
<b>Other standards and guidelines</b>	<ul style="list-style-type: none"> <li>■ EN 60529 Degrees of protection provided by enclosures (IP code)</li> <li>■ EN 61010-1 Safety requirements for electrical equipment for measurement, control and laboratory use - general requirements</li> <li>■ IEC/EN 61326 Emission in accordance with Class A requirements. Electromagnetic compatibility (EMC requirements).</li> <li>■ NAMUR NE 21 Electromagnetic compatibility (EMC) of industrial process and laboratory control equipment</li> <li>■ NAMUR NE 32 Data retention in the event of a power failure in field and control instruments with microprocessors</li> <li>■ NAMUR NE 43 Standardization of the signal level for the breakdown information of digital transmitters with analog output signal.</li> <li>■ NAMUR NE 53 Software of field devices and signal-processing devices with digital electronics</li> <li>■ NAMUR NE 105 Specifications for integrating fieldbus devices in engineering tools for field devices</li> <li>■ NAMUR NE 107 Self-monitoring and diagnosis of field devices</li> </ul>

- NAMUR NE 131  
Requirements for field devices for standard applications
- ETSI EN 300 328  
Guidelines for 2.4 GHz radio components.
- EN 301489  
Electromagnetic compatibility and radio spectrum matters (ERM).

## Ordering information

Detailed ordering information is available from the following sources:

- In the Product Configurator on the Endress+Hauser website: [www.endress.com](http://www.endress.com) -> Click "Corporate" -> Select your country -> Click "Products" -> Select the product using the filters and search field -> Open product page -> The "Configure" button to the right of the product image opens the Product Configurator.
- From your Endress+Hauser Sales Center: [www.addresses.endress.com](http://www.addresses.endress.com)



### Product Configurator - the tool for individual product configuration

- Up-to-the-minute configuration data
- Depending on the device: Direct input of measuring point-specific information such as measuring range or operating language
- Automatic verification of exclusion criteria
- Automatic creation of the order code and its breakdown in PDF or Excel output format
- Ability to order directly in the Endress+Hauser Online Shop



## Application packages

Many different application packages are available to enhance the functionality of the device. Such packages might be needed to address safety aspects or specific application requirements.

The application packages can be ordered with the device or subsequently from Endress+Hauser. Detailed information on the order code in question is available from your local Endress+Hauser sales center or on the product page of the Endress+Hauser website: [www.endress.com](http://www.endress.com).



### Diagnostics functions








Package	Description
Extended HistoROM	<p>Comprises extended functions concerning the event log and the activation of the measured value memory.</p> <p>Event log: Memory volume is extended from 20 message entries (standard version) to up to 100 entries.</p> <p>Data logging (line recorder):</p> <ul style="list-style-type: none"> <li>■ Memory capacity for up to 1000 measured values is activated.</li> <li>■ 250 measured values can be output via each of the 4 memory channels. The recording interval can be defined and configured by the user.</li> <li>■ Measured value logs can be accessed via the local display or operating tool e.g. FieldCare, DeviceCare or Web server.</li> </ul>

Heartbeat Technology	Package	Description
	Heartbeat Verification +Monitoring	<p><b>Heartbeat Verification</b> Meets the requirement for traceable verification to DIN ISO 9001:2008 Chapter 7.6 a) "Control of monitoring and measuring equipment".</p> <ul style="list-style-type: none"> <li>■ Functional testing in the installed state without interrupting the process.</li> <li>■ Traceable verification results on request, including a report.</li> <li>■ Simple testing process via local operation or other operating interfaces.</li> <li>■ Clear measuring point assessment (pass/fail) with high test coverage within the framework of manufacturer specifications.</li> <li>■ Extension of calibration intervals according to operator's risk assessment.</li> </ul> <p><b>Heartbeat Monitoring</b> Continuously supplies data, which are characteristic of the measuring principle, to an external condition monitoring system for the purpose of preventive maintenance or process analysis. These data enable the operator to:</p> <ul style="list-style-type: none"> <li>■ Draw conclusions - using these data and other information - about the impact process influences (such as corrosion, abrasion, buildup etc.) have on the measuring performance over time.</li> <li>■ Schedule servicing in time.</li> <li>■ Monitor the process or product quality, e.g. gas pockets.</li> </ul>
Cleaning	Package	Description
	Electrode cleaning circuit (ECC)	The electrode cleaning circuit (ECC) function has been developed to have a solution for applications where magnetite ( $\text{Fe}_3\text{O}_4$ ) deposits frequently occur (e.g. hot water). Since magnetite is highly conductive this build up leads to measuring errors and ultimately to the loss of signal. The application package is designed to AVOID build up of highly conductive matter and thin layers (typical of magnetite).
OPC-UA server	Package	Description
	OPC-UA-Server	<p>The application package provides the user with an integrated OPC-UA server for comprehensive instrument services for IoT and SCADA applications.</p> <p> Special Documentation for the "OPC-UA-Server" application package →  110.</p>


## Accessories

Various accessories, which can be ordered with the device or subsequently from Endress+Hauser, are available for the device. Detailed information on the order code in question is available from your local Endress+Hauser sales center or on the product page of the Endress+Hauser website: [www.endress.com](http://www.endress.com).


Device-specific accessories	For the transmitter	
	Accessories	Description
	Transmitter Promag 300	<p>Transmitter for replacement or storage. Use the order code to define the following specifications:</p> <ul style="list-style-type: none"> <li>■ Approvals</li> <li>■ Output</li> <li>■ Input</li> <li>■ Display / operation</li> <li>■ Housing</li> <li>■ Software</li> </ul> <p> Order code: 5X3BXX</p> <p> For details, see Installation Instructions EA01150</p>






Remote display and operating module DKX001	<ul style="list-style-type: none"> <li>■ If ordered directly with the measuring device: Order code for "Display; operation", option <b>O</b> "Separate 4-line display, illum.; 10 m (30 ft)Cable; touch control".</li> <li>■ If ordered separately: <ul style="list-style-type: none"> <li>– Measuring device: order code for "Display; operation", option <b>M</b> "None, prepared for separate display".</li> <li>– DKX001: Via the separate product structure DKX001.</li> </ul> </li> <li>■ If ordered subsequently: DKX001: Via the separate product structure DKX001.</li> </ul> <p><b>Mounting bracket for DKX001</b></p> <ul style="list-style-type: none"> <li>■ Ordered directly with the DKX001: Order code for "Enclosed accessories", option <b>RA</b> "Mounting bracket, 1 1/2" pipe".</li> <li>■ If ordered subsequently: order number: 71340960</li> </ul> <p><b>Connecting cable (replacement cable)</b> Via the separate product structure: DKX002</p> <p> Further information on display and operating module DKX001 →  91.</p> <p> For details, see Special Documentation SD01763D</p>
External WLAN antenna	<p>External WLAN antenna with 2 m (6.6 ft)connecting cable and two angle brackets. Order code for "Enclosed accessories", option <b>P8</b> "Wireless antenna wide area".</p> <p> Further information on the WLAN interface →  97.</p>
Protective cover	<p>Is used to protect the measuring device from the effects of the weather: e.g. rainwater, excess heating from direct sunlight.</p> <p> Order number: 71343505</p> <p> For details, see Installation Instructions EA01160</p>

#### For the sensor



Accessories	Description
Adapter set	<p>Adapter connections for installing a Promag H instead of a Promag 30/33 A or Promag 30/33 H (DN 25).</p> <p>Consists of:</p> <ul style="list-style-type: none"> <li>■ 2 process connections</li> <li>■ Screws</li> <li>■ Seals</li> </ul>
Seal set	For the regular replacement of seals for the sensor.
Spacer	If replacing a DN 80/100 sensor in an existing installation, a spacer is needed if the new sensor is shorter.
Welding jig	Welding nipple as process connection: welding jig for installation in pipe.
Grounding rings	<p>Are used to ground the medium in lined measuring tubes to ensure proper measurement.</p> <p> For details, see Installation Instructions EA00070D</p>
Mounting kit	<p>Consists of:</p> <ul style="list-style-type: none"> <li>■ 2 process connections</li> <li>■ Screws</li> <li>■ Seals</li> </ul>
Wall mounting kit	Wall mounting kit for measuring device (only DN 2 to 25 (1/12 to 1"))

#### Communication-specific accessories

Accessories	Description
Commubox FXA195 HART	<p>For intrinsically safe HART communication with FieldCare via the USB interface.</p> <p> For details, see "Technical Information" TI00404F</p>


HART Loop Converter HMX50	Is used to evaluate and convert dynamic HART process variables to analog current signals or limit values.  For details, see "Technical Information" TI00429F and Operating Instructions BA00371F
Fieldgate FXA320	Gateway for the remote monitoring of connected 4 to 20 mA measuring devices via a Web browser.  For details, see "Technical Information" TI00025S and Operating Instructions BA00053S
Fieldgate FXA520	Gateway for the remote diagnostics and remote configuration of connected HART measuring devices via a Web browser.  For details, see "Technical Information" TI00025S and Operating Instructions BA00051S
Field Xpert SFX350	Field Xpert SFX350 is a mobile computer for commissioning and maintenance. It enables efficient device configuration and diagnostics for HART and FOUNDATION Fieldbus devices and can be used in non-hazardous areas.  For details, see Operating Instructions BA01202S
Field Xpert SFX370	Field Xpert SFX370 is a mobile computer for commissioning and maintenance. It enables efficient device configuration and diagnostics for HART and FOUNDATION Fieldbus devices and can be used in the non-hazardous area and in the hazardous area.  For details, see Operating Instructions BA01202S

## Service-specific accessories

Accessories	Description
Applicator	Software for selecting and sizing Endress+Hauser measuring devices: <ul style="list-style-type: none"> <li>Choice of measuring devices for industrial requirements</li> <li>Calculation of all the necessary data for identifying the optimum flowmeter: e.g. nominal diameter, pressure loss, flow velocity and accuracy.</li> <li>Graphic illustration of the calculation results</li> <li>Determination of the partial order code, administration, documentation and access to all project-related data and parameters over the entire life cycle of a project.</li> </ul> Applicator is available: <ul style="list-style-type: none"> <li>Via the Internet: <a href="https://wapps.endress.com/applicator">https://wapps.endress.com/applicator</a></li> <li>As a downloadable DVD for local PC installation.</li> </ul>
W@M	W@M Life Cycle Management Improved productivity with information at your fingertips. Data relevant to a plant and its components is generated from the first stages of planning and during the asset's complete life cycle. W@M Life Cycle Management is an open and flexible information platform with online and on-site tools. Instant access for your staff to current, in-depth data shortens your plant's engineering time, speeds up procurement processes and increases plant uptime. Combined with the right services, W@M Life Cycle Management boosts productivity in every phase. For more information, visit <a href="http://www.endress.com/lifecyclemanagement">www.endress.com/lifecyclemanagement</a>
FieldCare	FDT-based plant asset management tool from Endress+Hauser. It can configure all smart field units in your system and helps you manage them. By using the status information, it is also a simple but effective way of checking their status and condition.  For details, see Operating Instructions BA00027S and BA00059S
DeviceCare	Tool for connecting and configuring Endress+Hauser field devices.  For details, see Innovation brochure IN01047S



## System components

Accessories	Description
Memograph M graphic data manager	The Memograph M graphic data manager provides information on all the relevant measured variables. Measured values are recorded correctly, limit values are monitored and measuring points analyzed. The data are stored in the 256 MB internal memory and also on a SD card or USB stick.  For details, see "Technical Information" TI00133R and Operating Instructions BA00247R

## Supplementary documentation



For an overview of the scope of the associated Technical Documentation, refer to the following:

- The *W@M Device Viewer* : Enter the serial number from the nameplate ([www.endress.com/deviceviewer](http://www.endress.com/deviceviewer))
- The *Endress+Hauser Operations App*: Enter the serial number from the nameplate or scan the 2-D matrix code (QR code) on the nameplate.

## Standard documentation

## Brief Operating Instructions

*Brief Operating Instructions for the sensor*

Measuring device	Documentation code
Proline Promag H	KA01289D

*Brief Operating Instructions for transmitter*

Measuring device	Documentation code					
	HART	FOUNDATION Fieldbus	PROFIBUS PA	Modbus RS485	EtherNet/IP	PROFINET
Proline 300	KA01308D	KA01294D	KA01227D	KA01310D	KA01338D	KA01340D

## Operating Instructions

Measuring device	Documentation code					
	HART	FOUNDATION Fieldbus	PROFIBUS PA	Modbus RS485	EtherNet/IP	PROFINET
Promag H 300	BA01392D	BA01477D	BA01396D	BA01394D	BA01716D	BA01718D

## Description of device parameters

Measuring device	Documentation code					
	HART	FOUNDATION Fieldbus	PROFIBUS PA	Modbus RS485	EtherNet/IP	PROFINET
Promag 300	GP01051D	GP01098D	GP01052D	GP01053D	GP01113D	GP01112D

## Device-dependent additional documentation

## Safety instructions

Safety instructions for electrical equipment for hazardous areas.

Contents	Documentation code
ATEX/IECEX Ex d/Ex de	XA01414D
ATEX/IECEX Ex ec	XA01514D
cCSAus XP	XA01515D
cCSAus Ex d/ Ex de	XA01516D

Contents	Documentation code
cCSAus Ex nA	XA01517D
INMETRO Ex d/Ex de	XA01518D
INMETRO Ex ec	XA01519D
NEPSI Ex d/Ex de	XA01520D
NEPSI Ex nA	XA01521D

#### Remote display and operating module DKX001

Contents	Documentation code
ATEX/IECEX Ex i	XA01494D
ATEX/IECEX Ex ec	XA01498D
cCSAus IS	XA01499D
cCSAus Ex nA	XA01513D
INMETRO Ex i	XA01500D
INMETRO Ex ec	XA01501D
NEPSI Ex i	XA01502D
NEPSI Ex nA	XA01503D

### Special Documentation

Contents	Documentation code
Information on the Pressure Equipment Directive	SD01614D
Functional Safety Manual	SD01740D
Radio approvals for WLAN interface for A309/A310 display module	SD01793D
Remote display and operating module DKX001	SD01763D
OPC-UA-Server <sup>1)</sup>	SD02043D

1) This Special Documentation is only available for device versions with a HART output.

Contents	Documentation code					
	HART	FOUNDATION Fieldbus	PROFIBUS PA	Modbus RS485	PROFINET	EtherNet/IP
Heartbeat Technology	SD01640D	SD01742D	SD01744D	SD01743D	SD01986D	SD01980D
Web server	SD01654D	SD01657D	SD01656D	SD01655D	SD01977D	SD01976D

### Installation Instructions

Contents	Comment
Installation instructions for spare part sets and accessories	Documentation code: specified for each individual accessory .

## Registered trademarks

### HART®

Registered trademark of the FieldComm Group, Austin, Texas, USA

### PROFIBUS®

Registered trademark of the PROFIBUS User Organization, Karlsruhe, Germany

**FOUNDATION™ Fieldbus**

Registration-pending trademark of the FieldComm Group, Austin, Texas, USA

**Modbus®**

Registered trademark of SCHNEIDER AUTOMATION, INC.

**EtherNet/IP™**

Trademark of ODVA, Inc.

**PROFINET®**

Registered trademark of the PROFIBUS User Organization, Karlsruhe, Germany

[www.addresses.endress.com](http://www.addresses.endress.com)

---